

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035467.D
 Acq On : 29 Apr 2024 13:45
 Operator : SY/MD
 Sample : P2279-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035467.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	50	54	63	rBV	8642	10448	0.58%	0.076%
2	1.278	67	74	92	rVB	255523	277049	15.27%	2.003%
3	1.529	146	152	167	rVB	188055	212301	11.70%	1.535%
4	2.053	306	315	331	rBV	430128	620602	34.21%	4.486%
5	2.487	448	450	453	rBV2	512	308	0.02%	0.002%
6	2.522	458	461	462	rBV	384	195	0.01%	0.001%
7	2.793	542	545	548	rBV2	272	180	0.01%	0.001%
8	2.915	581	583	589	rVB3	435	360	0.02%	0.003%
9	2.947	590	593	594	rBV2	212	103	0.01%	0.001%
10	3.008	609	612	618	rVB2	337	350	0.02%	0.003%
11	3.047	618	624	627	rBV4	352	375	0.02%	0.003%
12	3.072	629	632	643	rVB3	325	418	0.02%	0.003%
13	3.117	643	646	649	rBV	251	146	0.01%	0.001%
14	3.137	649	652	653	rBV	224	140	0.01%	0.001%
15	3.223	676	679	684	rVB	405	230	0.01%	0.002%
16	3.249	684	687	691	rBV2	220	169	0.01%	0.001%
17	3.275	691	695	698	rBV3	197	171	0.01%	0.001%
18	3.326	708	711	713	rBV2	278	122	0.01%	0.001%
19	3.339	713	715	716	rVV2	254	101	0.01%	0.001%
20	3.362	720	722	727	rVB2	277	135	0.01%	0.001%
21	3.413	735	738	741	rBV	135	110	0.01%	0.001%
22	3.448	745	749	753	rBV2	271	281	0.02%	0.002%
23	3.487	758	761	762	rBV	176	79	0.00%	0.001%
24	3.548	776	780	784	rBV	196	249	0.01%	0.002%
25	3.616	799	801	805	rVB	310	164	0.01%	0.001%
26	3.654	805	813	817	rVB2	262	276	0.02%	0.002%
27	3.680	817	821	822	rBV	103	69	0.00%	0.000%
28	3.690	822	824	826	rVB	197	80	0.00%	0.001%
29	3.712	826	831	833	rBV	240	222	0.01%	0.002%
30	3.799	849	858	915	rBV	119724	401266	22.12%	2.901%
31	4.246	983	997	1029	rBV	281167	718110	39.58%	5.191%
32	4.953	1201	1217	1256	rBV2	692896	1814152	100.00%	13.114%
33	5.426	1361	1364	1368	rBV2	516	531	0.03%	0.004%
34	5.532	1386	1397	1429	rBV	566524	1180774	65.09%	8.536%
35	5.837	1483	1492	1514	rVB3	8082	19791	1.09%	0.143%
36	5.985	1526	1538	1582	rBV	389214	814142	44.88%	5.885%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035467.D
 Acq On : 29 Apr 2024 13:45
 Operator : SY/MD
 Sample : P2279-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.342	1644	1649	1652	rBV4	508	523	0.03%	0.004%
38	6.413	1668	1671	1674	rBV3	186	131	0.01%	0.001%
39	6.439	1678	1679	1680	rBV3	132	42	0.00%	0.000%
40	6.455	1680	1684	1687	rVB2	326	227	0.01%	0.002%
41	6.477	1687	1691	1694	rBV2	436	399	0.02%	0.003%
42	6.506	1699	1700	1702	rBV2	198	56	0.00%	0.000%
43	6.516	1702	1703	1705	rVV2	122	51	0.00%	0.000%
44	6.526	1705	1706	1709	rVV	265	159	0.01%	0.001%
45	6.558	1712	1716	1722	rBV2	382	343	0.02%	0.002%
46	6.587	1724	1725	1727	rBV2	147	54	0.00%	0.000%
47	6.651	1743	1745	1746	rBV2	120	57	0.00%	0.000%
48	6.670	1749	1751	1753	rVV2	239	87	0.00%	0.001%
49	6.686	1753	1756	1759	rVV	353	249	0.01%	0.002%
50	6.783	1783	1786	1790	rBV	140	133	0.01%	0.001%
51	6.815	1794	1796	1799	rVB2	135	69	0.00%	0.000%
52	6.834	1799	1802	1804	rBV2	170	121	0.01%	0.001%
53	6.911	1816	1826	1863	rBV	194047	384380	21.19%	2.779%
54	7.243	1918	1929	1966	rBV	781595	1393925	76.84%	10.076%
55	7.554	2016	2026	2054	rBV	135153	258275	14.24%	1.867%
56	7.876	2123	2126	2127	rBV2	442	227	0.01%	0.002%
57	7.911	2134	2137	2144	rVB5	858	876	0.05%	0.006%
58	7.947	2144	2148	2151	rVV2	279	202	0.01%	0.001%
59	7.963	2151	2153	2158	rVB2	367	216	0.01%	0.002%
60	8.030	2165	2174	2223	rBV2	352124	829757	45.74%	5.998%
61	8.641	2362	2364	2365	rBV	370	110	0.01%	0.001%
62	8.744	2392	2396	2397	rBV3	323	213	0.01%	0.002%
63	8.783	2397	2408	2444	rBV	878424	1458923	80.42%	10.546%
64	9.059	2492	2494	2500	rBV5	687	568	0.03%	0.004%
65	9.104	2506	2508	2511	rBV3	406	185	0.01%	0.001%
66	9.394	2596	2598	2599	rBV3	203	74	0.00%	0.001%
67	9.435	2609	2611	2613	rBV2	181	95	0.01%	0.001%
68	9.468	2619	2621	2623	rVB	225	70	0.00%	0.001%
69	9.603	2660	2663	2666	rVB2	351	186	0.01%	0.001%
70	9.622	2667	2669	2671	rBV	266	80	0.00%	0.001%
71	9.696	2689	2692	2693	rBV	238	114	0.01%	0.001%
72	9.754	2707	2710	2711	rBV	237	108	0.01%	0.001%
73	9.767	2711	2714	2717	rBV2	384	288	0.02%	0.002%
74	9.805	2725	2726	2727	rBV2	222	75	0.00%	0.001%
75	9.921	2759	2762	2764	rVB2	542	237	0.01%	0.002%
76	9.937	2764	2767	2768	rBV2	168	107	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035467.D
 Acq On : 29 Apr 2024 13:45
 Operator : SY/MD
 Sample : P2279-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	10.030	2794	2796	2800	rVB2	222	103	0.01%	0.001%
78	10.152	2822	2834	2856	rBV	583572	930067	51.27%	6.723%
79	10.397	2906	2910	2913	rBV3	431	449	0.02%	0.003%
80	10.619	2975	2979	2983	rBV3	323	310	0.02%	0.002%
81	10.702	3003	3005	3009	rVB	321	139	0.01%	0.001%
82	10.799	3033	3035	3038	rVB	684	364	0.02%	0.003%
83	11.014	3099	3102	3103	rBV	179	103	0.01%	0.001%
84	11.127	3130	3137	3144	rBV4	2518	4199	0.23%	0.030%
85	11.185	3144	3155	3186	rVV	785018	1242100	68.47%	8.979%
86	11.503	3245	3254	3260	rBV4	7338	14222	0.78%	0.103%
87	11.557	3261	3271	3304	rVB	750438	1222718	67.40%	8.839%
88	12.307	3501	3504	3507	rBV	423	281	0.02%	0.002%
89	12.374	3523	3525	3530	rVB2	635	336	0.02%	0.002%
90	12.995	3716	3718	3722	rBV2	617	324	0.02%	0.002%
91	13.204	3775	3783	3795	rBV3	6634	11727	0.65%	0.085%




Sum of corrected areas: 13833633

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035467.D
Acq On : 29 Apr 2024 13:45
Operator : SY/MD
Sample : P2279-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

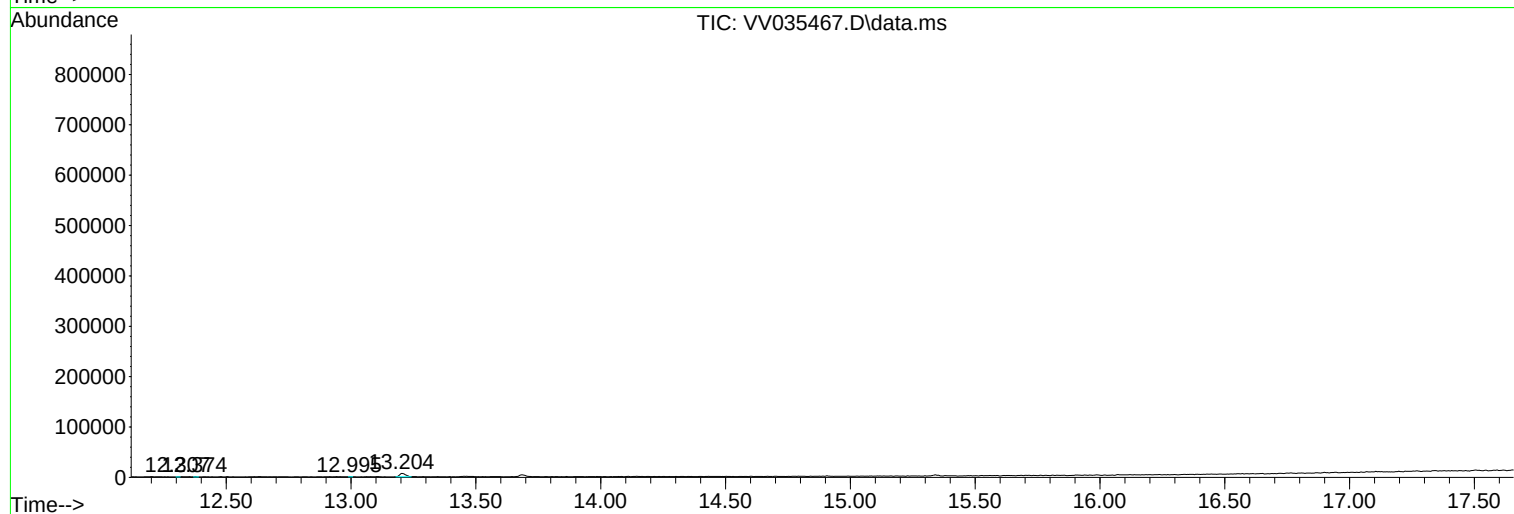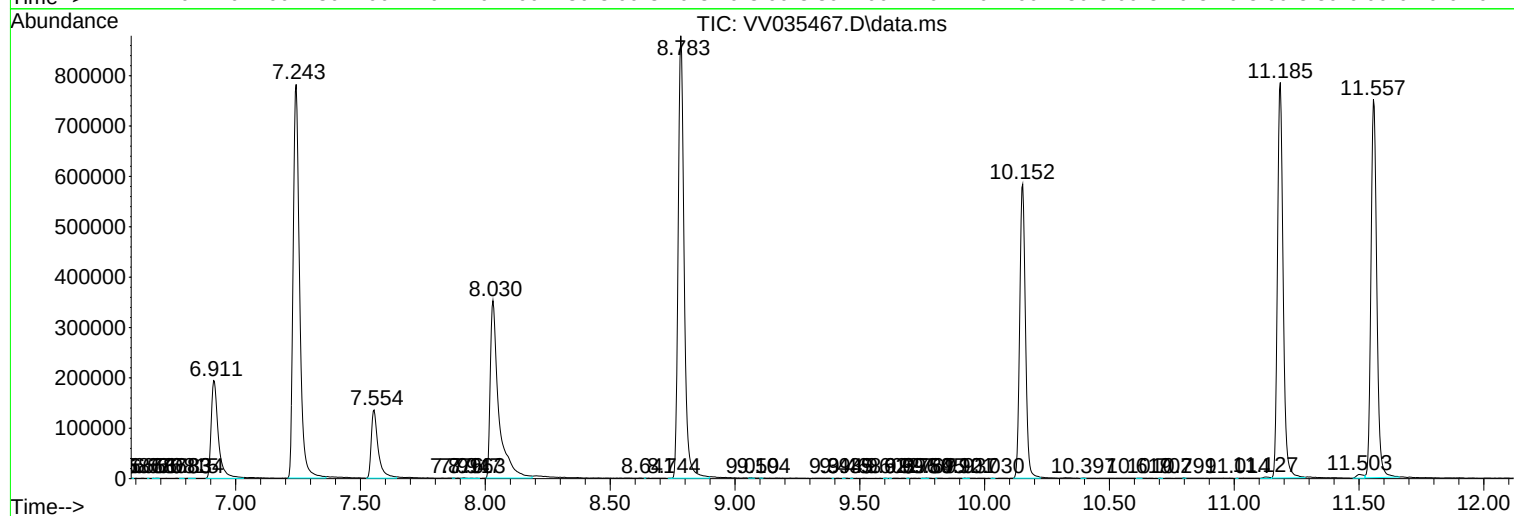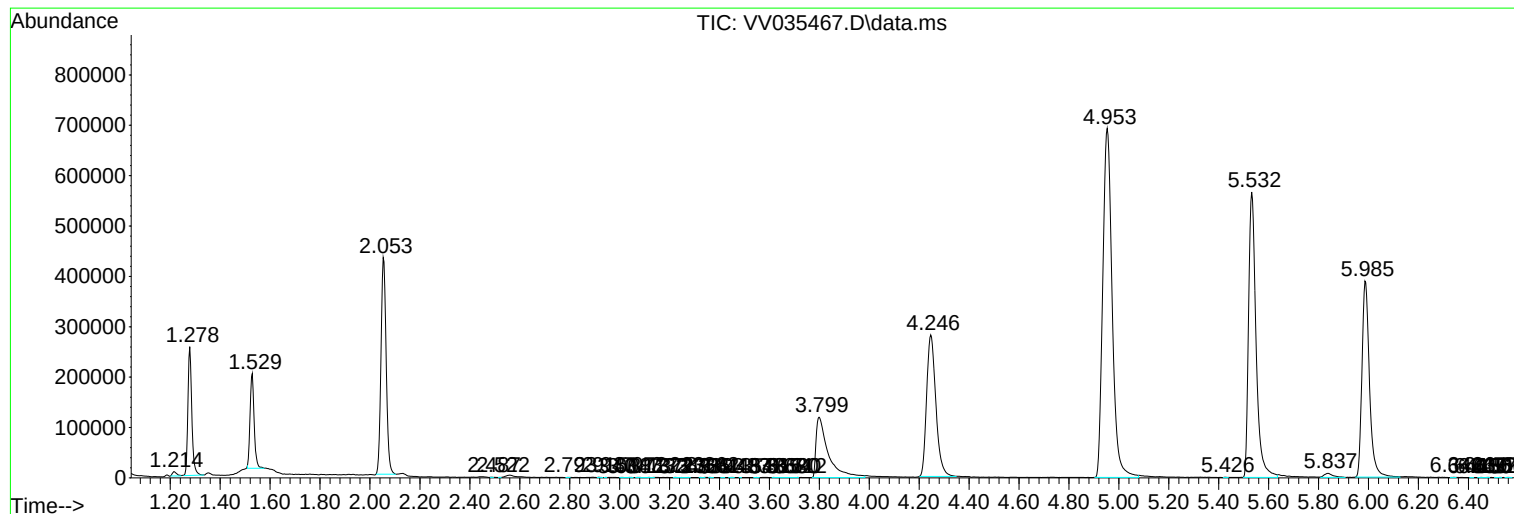

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035467.D
Acq On : 29 Apr 2024 13:45
Operator : SY/MD
Sample : P2279-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035467.D
Acq On : 29 Apr 2024 13:45
Operator : SY/MD
Sample : P2279-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc