

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035470.D
 Acq On : 29 Apr 2024 14:57
 Operator : SY/MD
 Sample : P2279-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	41	46	49	rBV	2448	2543	0.15%	0.019%
2	1.214	49	54	65	rVV	8147	11510	0.67%	0.084%
3	1.275	66	73	91	rVV	233563	257895	14.99%	1.892%
4	1.526	145	151	161	rVB	167091	185195	10.76%	1.358%
5	2.053	305	315	331	rBV	406959	591009	34.35%	4.335%
6	2.243	366	374	385	rVB3	2393	4464	0.26%	0.033%
7	2.378	414	416	421	rVB4	471	315	0.02%	0.002%
8	2.442	433	436	437	rBV2	994	519	0.03%	0.004%
9	2.510	455	457	459	rBV2	477	273	0.02%	0.002%
10	2.558	459	472	482	rBV	17013	37347	2.17%	0.274%
11	2.905	577	580	583	rBV	361	259	0.02%	0.002%
12	2.941	587	591	593	rBV	403	240	0.01%	0.002%
13	3.085	630	636	641	rBV3	402	452	0.03%	0.003%
14	3.117	641	646	649	rBV2	242	237	0.01%	0.002%
15	3.265	687	692	696	rVB2	292	279	0.02%	0.002%
16	3.625	801	804	808	rVB3	378	252	0.01%	0.002%
17	3.693	820	825	828	rBV2	356	295	0.02%	0.002%
18	3.799	849	858	901	rBV	113689	387997	22.55%	2.846%
19	4.246	980	997	1033	rBV	269421	697648	40.55%	5.118%
20	4.953	1201	1217	1266	rBV2	655164	1720456	100.00%	12.620%
21	5.275	1313	1317	1320	rBV2	337	266	0.02%	0.002%
22	5.313	1325	1329	1331	rBV2	347	255	0.01%	0.002%
23	5.384	1349	1351	1356	rBV	327	256	0.01%	0.002%
24	5.532	1385	1397	1446	rBV	542386	1147304	66.69%	8.416%
25	5.834	1481	1491	1501	rBV7	4061	8908	0.52%	0.065%
26	5.908	1513	1514	1520	rVB3	437	280	0.02%	0.002%
27	5.934	1520	1522	1524	rBV2	680	398	0.02%	0.003%
28	5.985	1524	1538	1568	rBV	375898	778810	45.27%	5.713%
29	6.233	1612	1615	1619	rVB4	522	342	0.02%	0.003%
30	6.288	1628	1632	1635	rBV3	644	536	0.03%	0.004%
31	6.349	1648	1651	1655	rVV3	595	422	0.02%	0.003%
32	6.371	1655	1658	1663	rVB4	459	324	0.02%	0.002%
33	6.474	1687	1690	1693	rBV2	365	234	0.01%	0.002%
34	6.677	1749	1753	1757	rVB2	398	323	0.02%	0.002%
35	6.702	1757	1761	1763	rBV2	480	335	0.02%	0.002%
36	6.812	1792	1795	1799	rBV2	276	243	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035470.D
 Acq On : 29 Apr 2024 14:57
 Operator : SY/MD
 Sample : P2279-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.854	1803	1808	1811	rBV2	220	240	0.01%	0.002%
38	6.911	1815	1826	1853	rBV	178552	350770	20.39%	2.573%
39	7.243	1917	1929	1967	rBV	728430	1297608	75.42%	9.519%
40	7.554	2016	2026	2058	rBV	125013	241261	14.02%	1.770%
41	7.870	2120	2124	2127	rVV4	474	330	0.02%	0.002%
42	7.989	2157	2161	2165	rVB	374	331	0.02%	0.002%
43	8.030	2165	2174	2214	rBV2	335037	795442	46.23%	5.835%
44	8.188	2216	2223	2246	rVB3	23775	55395	3.22%	0.406%
45	8.577	2340	2344	2347	rBV3	348	295	0.02%	0.002%
46	8.612	2352	2355	2358	rBV3	354	267	0.02%	0.002%
47	8.722	2386	2389	2392	rVB2	417	243	0.01%	0.002%
48	8.783	2397	2408	2438	rBV	856604	1533796	89.15%	11.251%
49	8.976	2466	2468	2471	rBV3	572	358	0.02%	0.003%
50	9.149	2519	2522	2524	rBV3	553	265	0.02%	0.002%
51	9.294	2564	2567	2571	rBV3	442	332	0.02%	0.002%
52	9.336	2577	2580	2585	rVV2	375	252	0.01%	0.002%
53	9.381	2590	2594	2598	rBV2	307	236	0.01%	0.002%
54	9.458	2614	2618	2620	rBV2	435	330	0.02%	0.002%
55	9.484	2621	2626	2631	rBV3	314	378	0.02%	0.003%
56	9.789	2717	2721	2724	rBV3	464	429	0.02%	0.003%
57	9.802	2724	2725	2729	rVB2	559	321	0.02%	0.002%
58	9.866	2743	2745	2748	rBV	410	272	0.02%	0.002%
59	9.902	2753	2756	2759	rVB2	335	238	0.01%	0.002%
60	9.924	2759	2763	2767	rBV2	347	321	0.02%	0.002%
61	10.075	2806	2810	2813	rBV2	370	280	0.02%	0.002%
62	10.152	2821	2834	2861	rBV	580634	926949	53.88%	6.800%
63	10.326	2886	2888	2894	rVB4	1033	868	0.05%	0.006%
64	10.448	2925	2926	2932	rVB3	301	241	0.01%	0.002%
65	10.503	2933	2943	2947	rBV2	351	557	0.03%	0.004%
66	10.789	3029	3032	3035	rBV3	379	276	0.02%	0.002%
67	10.873	3053	3058	3062	rBV2	362	281	0.02%	0.002%
68	10.953	3081	3083	3089	rVV2	356	266	0.02%	0.002%
69	11.046	3109	3112	3118	rBV	212	232	0.01%	0.002%
70	11.123	3127	3136	3145	rBV3	19511	31340	1.82%	0.230%
71	11.185	3145	3155	3192	rVB	778277	1334388	77.56%	9.788%
72	11.487	3246	3249	3252	rBV2	470	284	0.02%	0.002%
73	11.558	3255	3271	3299	rBV	721454	1205113	70.05%	8.840%
74	11.837	3357	3358	3363	rVB2	639	343	0.02%	0.003%
75	11.992	3402	3406	3408	rBV2	389	264	0.02%	0.002%
76	12.069	3426	3430	3434	rBV3	539	451	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035470.D
 Acq On : 29 Apr 2024 14:57
 Operator : SY/MD
 Sample : P2279-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	12.178	3461	3464	3466	rBV3	502	263	0.02%	0.002%
78	12.239	3481	3483	3488	rVB2	370	248	0.01%	0.002%
79	12.287	3494	3498	3500	rBV2	416	272	0.02%	0.002%
80	12.310	3500	3505	3507	rBV4	828	860	0.05%	0.006%
81	12.355	3516	3519	3523	rBV4	499	353	0.02%	0.003%
82	12.439	3543	3545	3550	rVB	430	260	0.02%	0.002%
83	12.467	3550	3554	3556	rBV	419	304	0.02%	0.002%
84	12.557	3575	3582	3585	rBV2	542	653	0.04%	0.005%
85	12.586	3588	3591	3595	rVV3	400	373	0.02%	0.003%
86	12.773	3644	3649	3651	rBV2	456	441	0.03%	0.003%
87	12.885	3678	3684	3687	rBV2	580	548	0.03%	0.004%
88	12.975	3709	3712	3716	rBV2	323	289	0.02%	0.002%
89	13.046	3731	3734	3736	rBV2	434	254	0.01%	0.002%
90	13.066	3736	3740	3744	rBV3	561	569	0.03%	0.004%
91	13.101	3748	3751	3753	rBV	375	267	0.02%	0.002%
92	13.207	3779	3784	3792	rVV3	2123	3070	0.18%	0.023%
93	13.422	3847	3851	3853	rBV3	324	308	0.02%	0.002%
94	13.683	3929	3932	3934	rBV	474	321	0.02%	0.002%
95	13.959	4016	4018	4025	rVB3	403	306	0.02%	0.002%
96	14.120	4065	4068	4071	rBV2	459	397	0.02%	0.003%
97	14.172	4078	4084	4087	rBV3	518	667	0.04%	0.005%
98	14.246	4104	4107	4109	rBV2	636	337	0.02%	0.002%
99	14.432	4164	4165	4170	rBV3	526	333	0.02%	0.002%
100	14.795	4275	4278	4281	rBV3	576	384	0.02%	0.003%




Sum of corrected areas: 13632341

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035470.D
Acq On : 29 Apr 2024 14:57
Operator : SY/MD
Sample : P2279-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

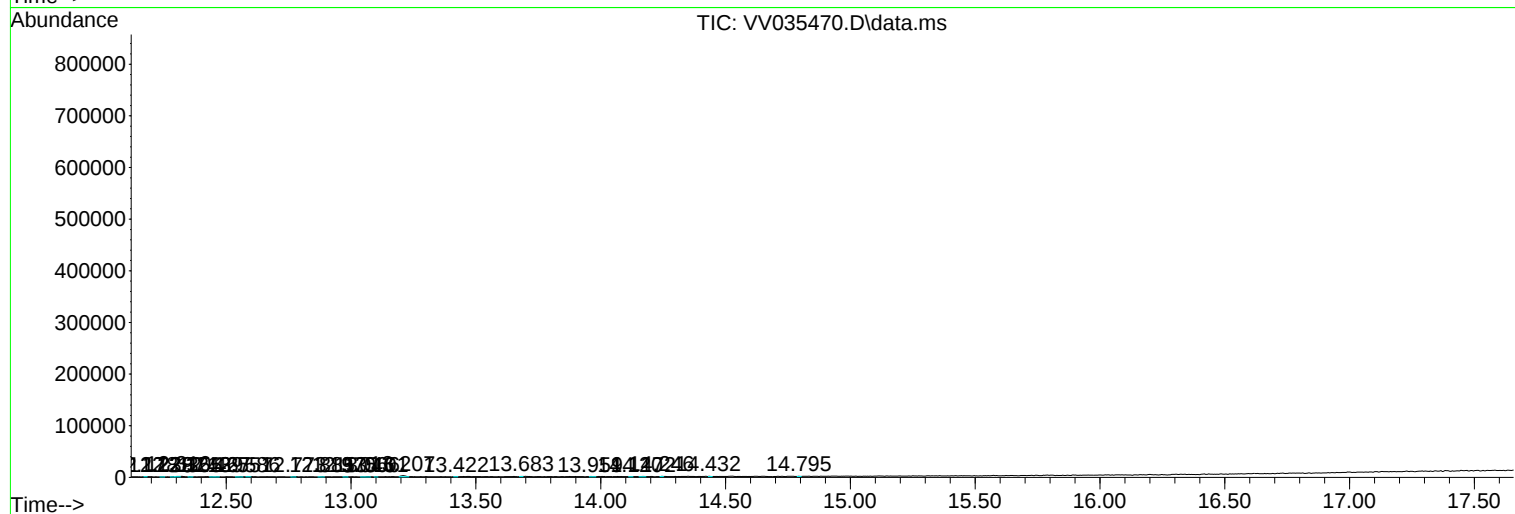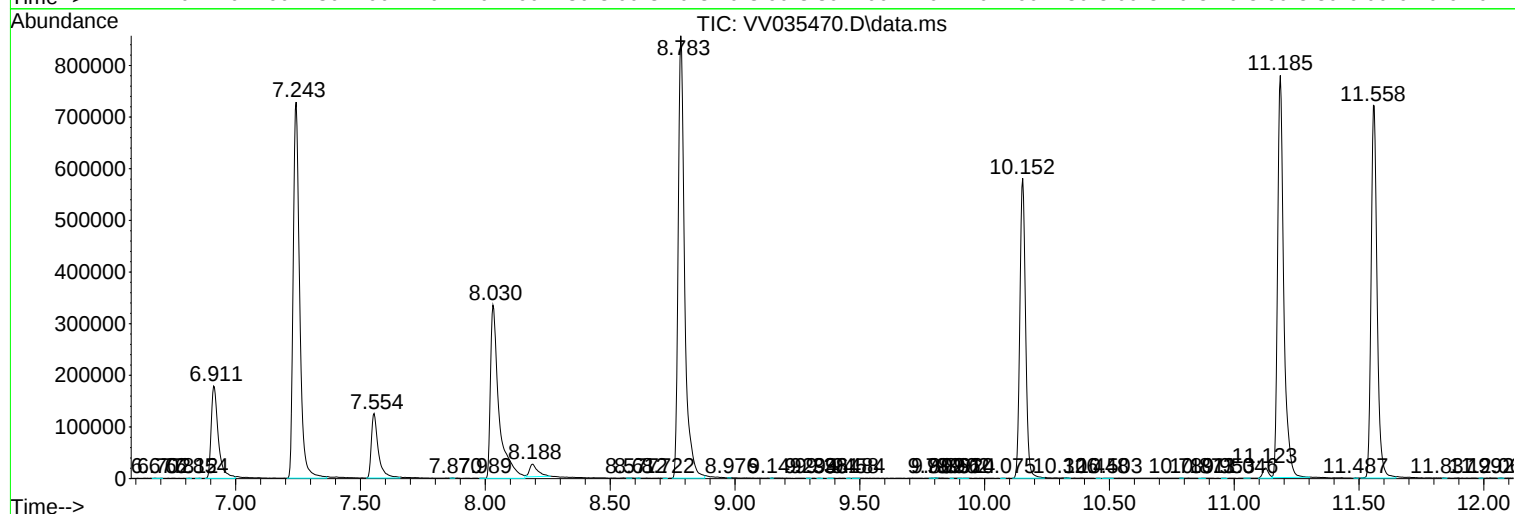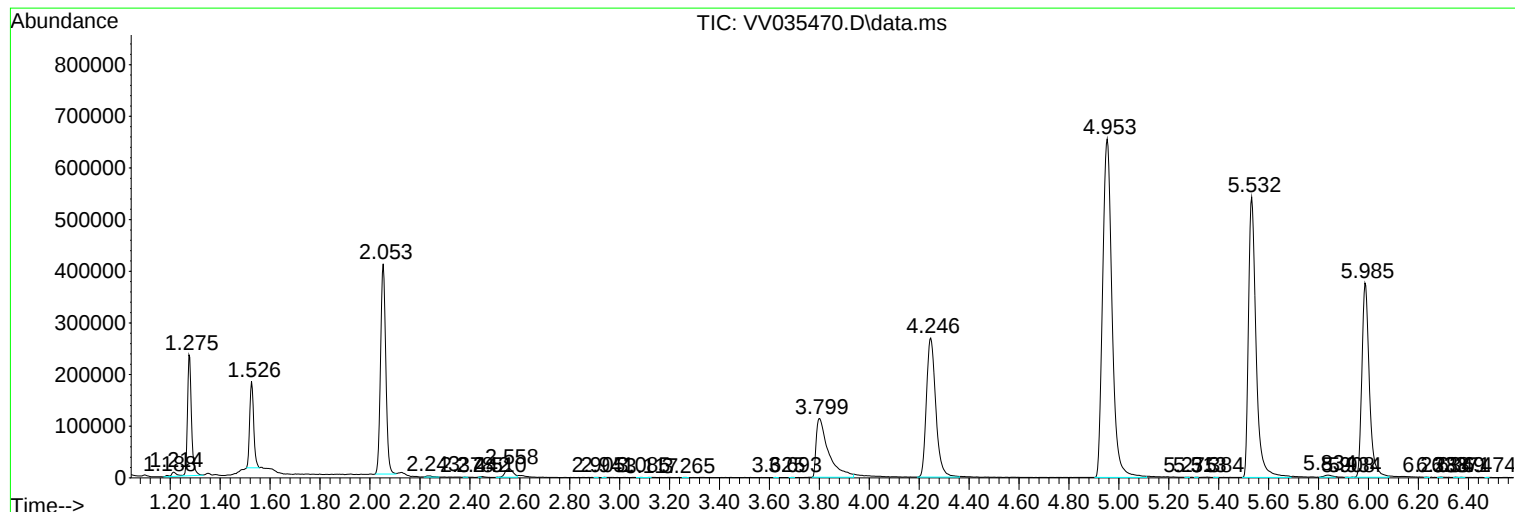

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035470.D
Acq On : 29 Apr 2024 14:57
Operator : SY/MD
Sample : P2279-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035470.D
Acq On : 29 Apr 2024 14:57
Operator : SY/MD
Sample : P2279-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc