

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035471.D
 Acq On : 29 Apr 2024 15:21
 Operator : SY/MD
 Sample : P2269-05DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	41	45	49	rBV	2169	2232	0.10%	0.015%
2	1.214	50	54	60	rVV4	2536	3312	0.15%	0.022%
3	1.278	66	74	88	rBV	244660	265178	12.21%	1.730%
4	1.529	145	152	166	rBV	212369	237996	10.96%	1.552%
5	2.053	305	315	331	rBV	419268	606307	27.91%	3.955%
6	2.400	419	423	427	rBV3	494	493	0.02%	0.003%
7	2.442	430	436	449	rVB5	3357	5762	0.27%	0.038%
8	2.510	455	457	460	rBV2	371	259	0.01%	0.002%
9	2.558	460	472	481	rBV	5124	9822	0.45%	0.064%
10	2.735	523	527	533	rVV4	323	412	0.02%	0.003%
11	2.773	536	539	544	rBV	362	411	0.02%	0.003%
12	2.809	547	550	554	rVB2	312	203	0.01%	0.001%
13	2.834	554	558	559	rBV2	302	227	0.01%	0.001%
14	2.860	562	566	570	rVB2	306	237	0.01%	0.002%
15	2.883	570	573	579	rVB3	203	202	0.01%	0.001%
16	2.934	583	589	591	rBV	478	342	0.02%	0.002%
17	3.153	652	657	664	rVB2	293	399	0.02%	0.003%
18	3.233	679	682	688	rVB	266	254	0.01%	0.002%
19	3.268	688	693	698	rVB2	304	290	0.01%	0.002%
20	3.297	698	702	704	rBV2	280	222	0.01%	0.001%
21	3.484	755	760	764	rBV2	196	220	0.01%	0.001%
22	3.619	798	802	806	rVB	288	213	0.01%	0.001%
23	3.796	849	857	898	rBV	117591	377281	17.37%	2.461%
24	4.246	981	997	1027	rBV	277816	712107	32.78%	4.645%
25	4.426	1051	1053	1056	rBV	409	216	0.01%	0.001%
26	4.735	1142	1149	1150	rVV4	734	726	0.03%	0.005%
27	4.757	1154	1156	1161	rVB2	693	450	0.02%	0.003%
28	4.953	1201	1217	1232	rBV2	674197	1774955	81.71%	11.577%
29	5.301	1322	1325	1327	rBV2	342	243	0.01%	0.002%
30	5.326	1330	1333	1335	rBV2	391	296	0.01%	0.002%
31	5.371	1345	1347	1353	rVB3	644	398	0.02%	0.003%
32	5.461	1372	1375	1377	rBV2	403	249	0.01%	0.002%
33	5.532	1386	1397	1436	rBV	549621	1160092	53.40%	7.567%
34	5.760	1466	1468	1469	rBV	525	214	0.01%	0.001%
35	5.834	1481	1491	1512	rVB3	6631	16433	0.76%	0.107%
36	5.985	1526	1538	1582	rBV	380039	791683	36.44%	5.164%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035471.D
 Acq On : 29 Apr 2024 15:21
 Operator : SY/MD
 Sample : P2269-05DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.207	1606	1607	1611	rBV3	616	401	0.02%	0.003%
38	6.272	1624	1627	1630	rBV2	468	330	0.02%	0.002%
39	6.365	1655	1656	1659	rVB	437	205	0.01%	0.001%
40	6.394	1663	1665	1668	rBV2	318	226	0.01%	0.001%
41	6.464	1679	1687	1694	rVB5	612	771	0.04%	0.005%
42	6.648	1742	1744	1748	rVB	384	235	0.01%	0.002%
43	6.815	1792	1796	1798	rBV2	250	214	0.01%	0.001%
44	6.911	1816	1826	1853	rBV	179352	351153	16.16%	2.290%
45	7.243	1917	1929	1973	rBV	736753	1330012	61.23%	8.675%
46	7.452	1991	1994	1998	rVB3	741	603	0.03%	0.004%
47	7.554	2015	2026	2049	rBV	125237	237255	10.92%	1.547%
48	7.789	2097	2099	2102	rBV	379	262	0.01%	0.002%
49	7.873	2121	2125	2128	rVB3	412	336	0.02%	0.002%
50	8.027	2164	2173	2220	rBV2	353720	814161	37.48%	5.310%
51	8.368	2276	2279	2283	rVB5	1214	840	0.04%	0.005%
52	8.394	2283	2287	2288	rBV3	552	418	0.02%	0.003%
53	8.474	2310	2312	2318	rVB4	529	493	0.02%	0.003%
54	8.509	2318	2323	2327	rBV3	466	432	0.02%	0.003%
55	8.558	2335	2338	2343	rBV5	477	305	0.01%	0.002%
56	8.612	2349	2355	2356	rBV3	366	231	0.01%	0.002%
57	8.696	2378	2381	2385	rVB2	304	233	0.01%	0.002%
58	8.718	2385	2388	2393	rVB3	504	387	0.02%	0.003%
59	8.783	2393	2408	2412	rBV	929090	1365186	62.84%	8.904%
60	9.242	2548	2551	2553	rBV2	343	210	0.01%	0.001%
61	9.323	2572	2576	2578	rBV2	416	277	0.01%	0.002%
62	9.471	2620	2622	2627	rBV2	435	392	0.02%	0.003%
63	9.522	2636	2638	2641	rVB2	353	205	0.01%	0.001%
64	9.587	2654	2658	2662	rBV3	308	274	0.01%	0.002%
65	9.863	2742	2744	2750	rVB	274	208	0.01%	0.001%
66	9.947	2766	2770	2774	rBV2	245	278	0.01%	0.002%
67	10.062	2803	2806	2811	rVB3	377	280	0.01%	0.002%
68	10.152	2822	2834	2857	rBV	569442	908719	41.83%	5.927%
69	10.548	2953	2957	2960	rBV	415	278	0.01%	0.002%
70	10.680	2995	2998	3001	rVB2	331	219	0.01%	0.001%
71	10.699	3001	3004	3007	rBV2	344	266	0.01%	0.002%
72	10.734	3012	3015	3017	rBV2	318	235	0.01%	0.002%
73	10.792	3027	3033	3034	rBV4	411	333	0.02%	0.002%
74	10.914	3070	3071	3076	rVB2	383	203	0.01%	0.001%
75	11.120	3126	3135	3145	rBV	50507	81414	3.75%	0.531%
76	11.185	3145	3155	3192	rVB2	840020	1942618	89.43%	12.671%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035471.D
 Acq On : 29 Apr 2024 15:21
 Operator : SY/MD
 Sample : P2269-05DL 500X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

77	11.564	3258	3273	3298	rBV2	930812	2172311	100.00%	14.169%
78	11.783	3338	3341	3342	rBV2	465	290	0.01%	0.002%
79	11.860	3362	3365	3368	rBV3	414	265	0.01%	0.002%
80	11.972	3397	3400	3404	rBV3	352	297	0.01%	0.002%
81	12.037	3416	3420	3422	rBV	322	273	0.01%	0.002%
82	12.056	3423	3426	3428	rVB	404	226	0.01%	0.001%
83	12.194	3466	3469	3474	rBV2	389	437	0.02%	0.003%
84	12.512	3566	3568	3574	rVB2	479	399	0.02%	0.003%
85	12.548	3574	3579	3581	rBV3	361	314	0.01%	0.002%
86	12.818	3661	3663	3667	rVB2	510	336	0.02%	0.002%
87	12.908	3688	3691	3694	rBV3	361	314	0.01%	0.002%
88	12.959	3703	3707	3710	rBV	342	273	0.01%	0.002%
89	13.017	3721	3725	3729	rBV	296	257	0.01%	0.002%
90	13.152	3765	3767	3772	rVB2	487	337	0.02%	0.002%
91	13.201	3772	3782	3802	rBV2	69797	116852	5.38%	0.762%
92	13.451	3857	3860	3862	rBV4	521	409	0.02%	0.003%
93	13.609	3905	3909	3912	rVB2	380	217	0.01%	0.001%
94	13.686	3923	3933	3943	rBV2	14498	22962	1.06%	0.150%
95	13.786	3962	3964	3969	rVB3	550	412	0.02%	0.003%
96	14.072	4050	4053	4059	rBV2	705	449	0.02%	0.003%
97	14.310	4124	4127	4132	rBV2	819	572	0.03%	0.004%
98	14.609	4217	4220	4221	rBV2	474	231	0.01%	0.002%
99	14.789	4274	4276	4280	rVB4	746	460	0.02%	0.003%
100	14.975	4331	4334	4341	rBV3	860	1252	0.06%	0.008%




Sum of corrected areas: 15331579

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035471.D
Acq On : 29 Apr 2024 15:21
Operator : SY/MD
Sample : P2269-05DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

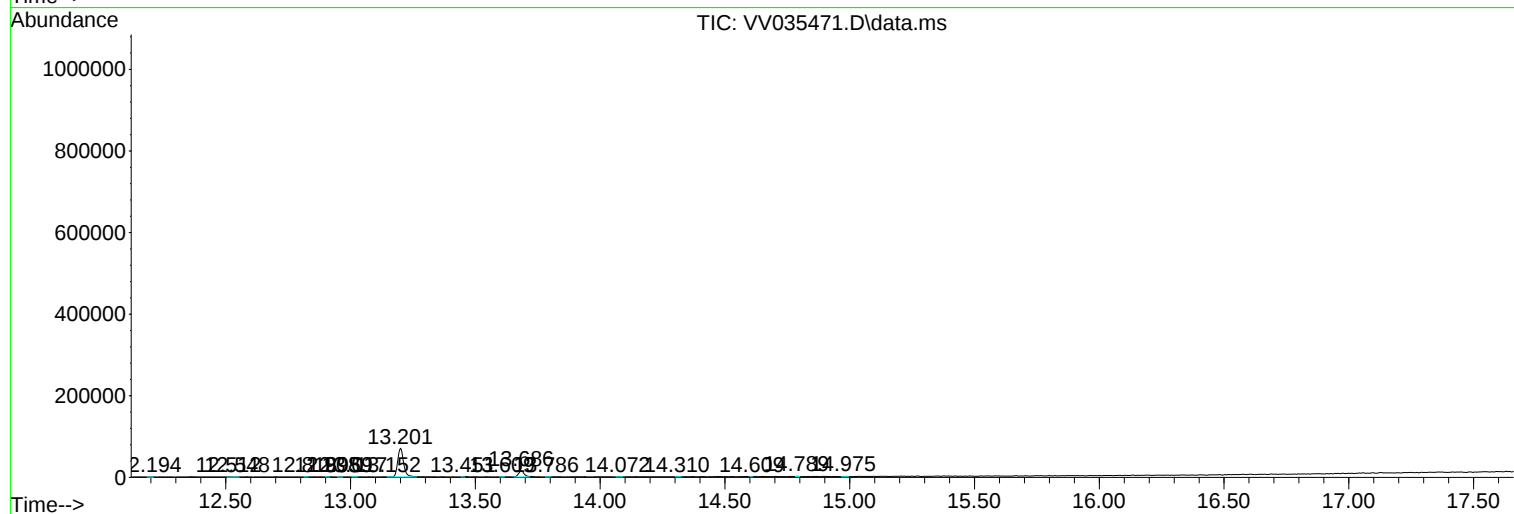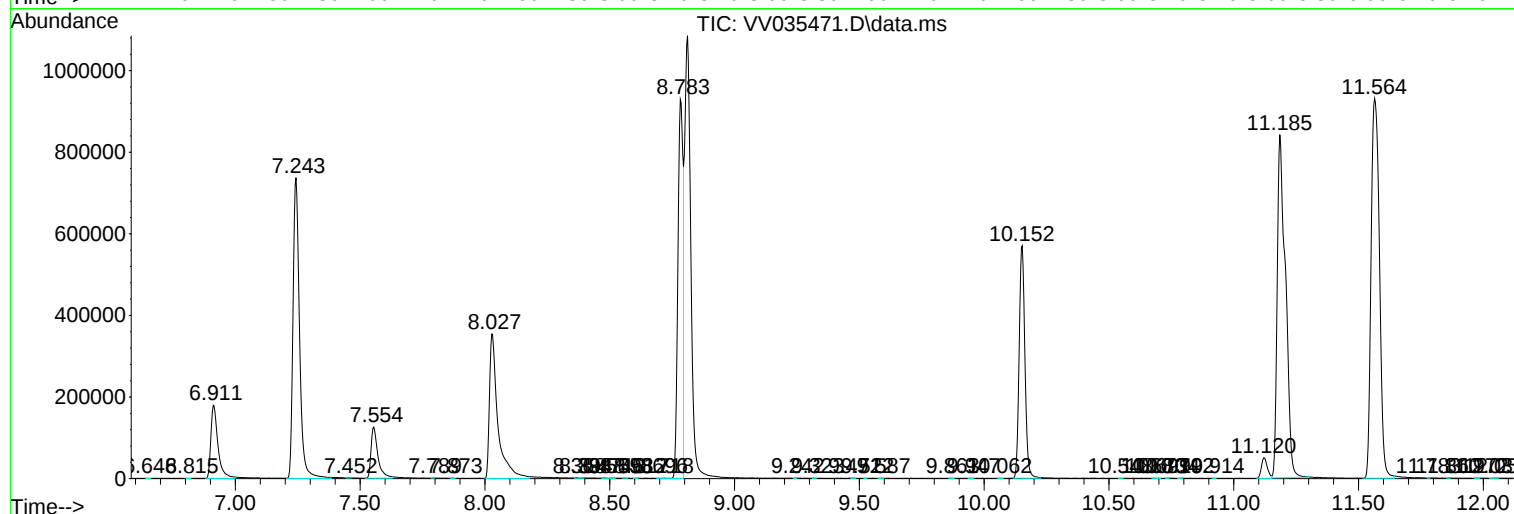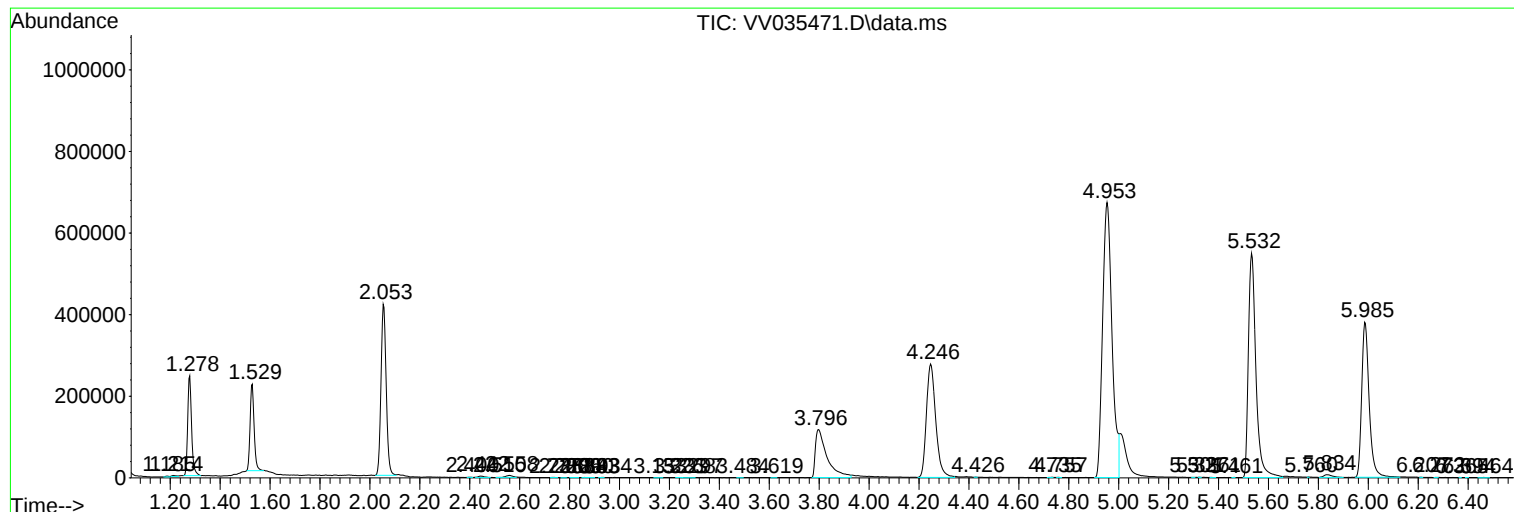

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035471.D
Acq On : 29 Apr 2024 15:21
Operator : SY/MD
Sample : P2269-05DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035471.D
Acq On : 29 Apr 2024 15:21
Operator : SY/MD
Sample : P2269-05DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------