

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035472.D
 Acq On : 29 Apr 2024 15:45
 Operator : SY/MD
 Sample : P2279-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035472.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	49	54	64	rBV	20355	24061	1.40%	0.182%
2	1.278	67	74	91	rVB	235951	258561	15.02%	1.951%
3	1.529	146	152	170	rVB	211784	241992	14.05%	1.826%
4	2.053	306	315	331	rBV	408745	585563	34.00%	4.419%
5	2.442	431	436	447	rVB5	1650	2535	0.15%	0.019%
6	2.555	461	471	493	rBV	21842	49557	2.88%	0.374%
7	2.822	552	554	556	rBV	207	94	0.01%	0.001%
8	2.899	575	578	580	rBV3	358	250	0.01%	0.002%
9	2.937	586	590	593	rBV2	310	197	0.01%	0.001%
10	2.966	598	599	602	rBV	187	119	0.01%	0.001%
11	2.992	602	607	614	rVB4	316	431	0.03%	0.003%
12	3.153	653	657	660	rVV2	295	256	0.01%	0.002%
13	3.169	660	662	665	rVB	177	84	0.00%	0.001%
14	3.211	672	675	680	rVB2	147	125	0.01%	0.001%
15	3.246	682	686	688	rBV	276	163	0.01%	0.001%
16	3.326	708	711	713	rVB2	227	111	0.01%	0.001%
17	3.404	732	735	737	rBV	177	108	0.01%	0.001%
18	3.471	748	756	759	rBV2	192	183	0.01%	0.001%
19	3.490	759	762	766	rBV2	128	117	0.01%	0.001%
20	3.523	771	772	775	rBV	258	91	0.01%	0.001%
21	3.542	775	778	782	rBV3	289	244	0.01%	0.002%
22	3.568	784	786	792	rVB	239	154	0.01%	0.001%
23	3.609	792	799	802	rBV	196	245	0.01%	0.002%
24	3.667	814	817	821	rVB2	180	141	0.01%	0.001%
25	3.712	828	831	833	rVB	237	140	0.01%	0.001%
26	3.725	833	835	838	rVB2	155	76	0.00%	0.001%
27	3.751	838	843	846	rBV2	113	105	0.01%	0.001%
28	3.799	849	858	903	rBV	118963	418034	24.28%	3.154%
29	4.246	982	997	1026	rBV	268671	691613	40.16%	5.219%
30	4.719	1142	1144	1148	rVB2	267	194	0.01%	0.001%
31	4.741	1148	1151	1152	rBV2	357	242	0.01%	0.002%
32	4.777	1157	1162	1165	rBV3	301	321	0.02%	0.002%
33	4.796	1165	1168	1170	rBV3	161	129	0.01%	0.001%
34	4.886	1194	1196	1198	rBV	272	135	0.01%	0.001%
35	4.953	1202	1217	1263	rBV2	654079	1722016	100.00%	12.994%
36	5.465	1374	1376	1377	rVB2	348	98	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035472.D
 Acq On : 29 Apr 2024 15:45
 Operator : SY/MD
 Sample : P2279-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1442	rBV	542233	1142287	66.33%	8.620%
38	5.841	1482	1493	1508	rBV4	6197	15239	0.88%	0.115%
39	5.986	1525	1538	1569	rBV	370758	771671	44.81%	5.823%
40	6.304	1634	1637	1638	rBV	451	266	0.02%	0.002%
41	6.336	1645	1647	1650	rVB2	315	142	0.01%	0.001%
42	6.352	1650	1652	1655	rBV	258	183	0.01%	0.001%
43	6.410	1667	1670	1673	rVB2	184	117	0.01%	0.001%
44	6.426	1673	1675	1679	rBV2	172	92	0.01%	0.001%
45	6.481	1690	1692	1695	rBV3	171	114	0.01%	0.001%
46	6.510	1699	1701	1704	rBV2	324	167	0.01%	0.001%
47	6.612	1731	1733	1737	rVB3	302	164	0.01%	0.001%
48	6.635	1737	1740	1742	rBV	217	125	0.01%	0.001%
49	6.706	1759	1762	1764	rBV3	207	142	0.01%	0.001%
50	6.735	1769	1771	1772	rBV2	257	78	0.00%	0.001%
51	6.793	1787	1789	1792	rVV	311	170	0.01%	0.001%
52	6.805	1792	1793	1796	rVB	328	116	0.01%	0.001%
53	6.876	1810	1815	1817	rBV2	440	329	0.02%	0.002%
54	6.912	1817	1826	1850	rBV	175003	344340	20.00%	2.598%
55	7.182	1908	1910	1912	rBV	521	211	0.01%	0.002%
56	7.243	1918	1929	1971	rBV	717351	1289463	74.88%	9.730%
57	7.555	2016	2026	2060	rBV	125213	238106	13.83%	1.797%
58	7.818	2106	2108	2110	rVB2	435	187	0.01%	0.001%
59	7.838	2110	2114	2119	rVB3	386	425	0.02%	0.003%
60	7.860	2119	2121	2123	rBV	511	267	0.02%	0.002%
61	7.960	2146	2152	2156	rBV4	604	469	0.03%	0.004%
62	7.982	2156	2159	2164	rBV3	190	152	0.01%	0.001%
63	8.030	2164	2174	2219	rBV3	337814	796509	46.25%	6.010%
64	8.532	2326	2330	2331	rBV3	357	227	0.01%	0.002%
65	8.583	2343	2346	2350	rVB3	663	397	0.02%	0.003%
66	8.641	2361	2364	2366	rBV	433	212	0.01%	0.002%
67	8.719	2386	2388	2390	rBV	534	269	0.02%	0.002%
68	8.783	2397	2408	2439	rBV	837079	1413944	82.11%	10.670%
69	9.095	2503	2505	2507	rVB3	507	205	0.01%	0.002%
70	9.194	2534	2536	2537	rVB	343	87	0.01%	0.001%
71	9.252	2549	2554	2561	rBV3	557	646	0.04%	0.005%
72	9.368	2586	2590	2594	rVB4	484	333	0.02%	0.003%
73	9.394	2596	2598	2600	rBV	216	118	0.01%	0.001%
74	9.410	2601	2603	2605	rVV2	307	130	0.01%	0.001%
75	9.516	2633	2636	2638	rBV	311	175	0.01%	0.001%
76	9.657	2678	2680	2683	rVB	262	133	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035472.D
 Acq On : 29 Apr 2024 15:45
 Operator : SY/MD
 Sample : P2279-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	9.686	2683	2689	2691	rBV2	353	354	0.02%	0.003%
78	9.715	2696	2698	2702	rVB2	368	226	0.01%	0.002%
79	9.735	2702	2704	2707	rBV	221	135	0.01%	0.001%
80	9.776	2714	2717	2721	rVB2	245	198	0.01%	0.001%
81	9.802	2721	2725	2727	rBV2	127	105	0.01%	0.001%
82	9.844	2735	2738	2740	rBV	218	145	0.01%	0.001%
83	9.854	2740	2741	2746	rVB	352	186	0.01%	0.001%
84	9.908	2752	2758	2761	rBV3	303	298	0.02%	0.002%
85	10.024	2791	2794	2798	rBV3	413	313	0.02%	0.002%
86	10.153	2821	2834	2862	rBV	558717	886517	51.48%	6.690%
87	10.368	2898	2901	2903	rBV2	391	287	0.02%	0.002%
88	10.526	2946	2950	2951	rBV2	368	204	0.01%	0.002%
89	10.606	2973	2975	2979	rBV2	391	193	0.01%	0.001%
90	10.741	3014	3017	3021	rBV	353	221	0.01%	0.002%
91	10.860	3051	3054	3058	rBV2	237	173	0.01%	0.001%
92	11.130	3132	3138	3144	rBV2	2426	3255	0.19%	0.025%
93	11.185	3144	3155	3180	rBV	725820	1175524	68.26%	8.870%
94	11.558	3256	3271	3296	rBV	702674	1156372	67.15%	8.726%
95	11.937	3385	3389	3390	rBV2	544	351	0.02%	0.003%
96	11.992	3403	3406	3408	rBV	287	178	0.01%	0.001%
97	12.191	3465	3468	3472	rBV	565	490	0.03%	0.004%
98	12.535	3571	3575	3584	rVV4	491	452	0.03%	0.003%
99	12.574	3584	3587	3592	rVB	471	329	0.02%	0.002%
100	13.207	3778	3784	3795	rVB4	5646	8718	0.51%	0.066%




Sum of corrected areas: 13252116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035472.D
Acq On : 29 Apr 2024 15:45
Operator : SY/MD
Sample : P2279-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

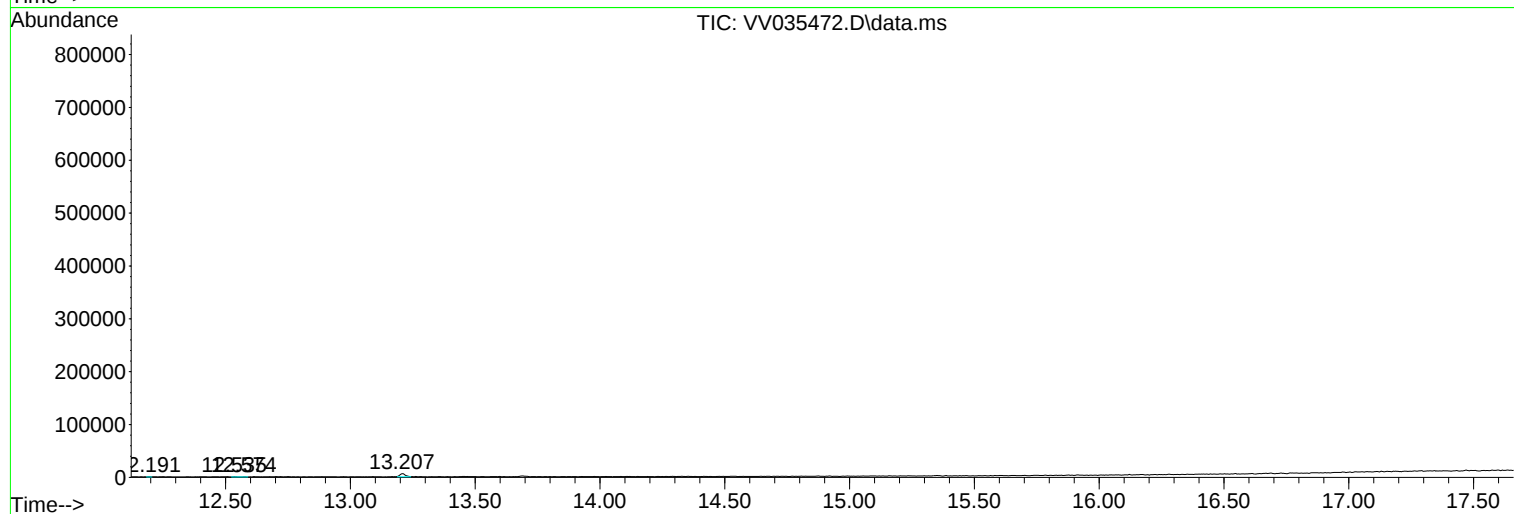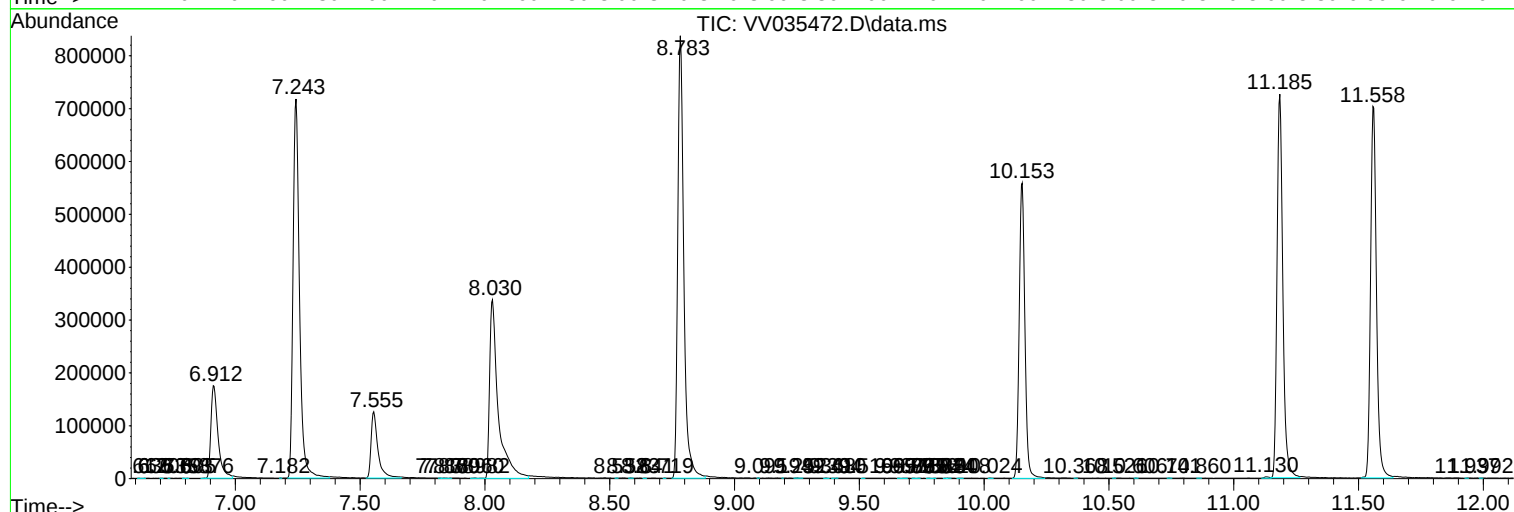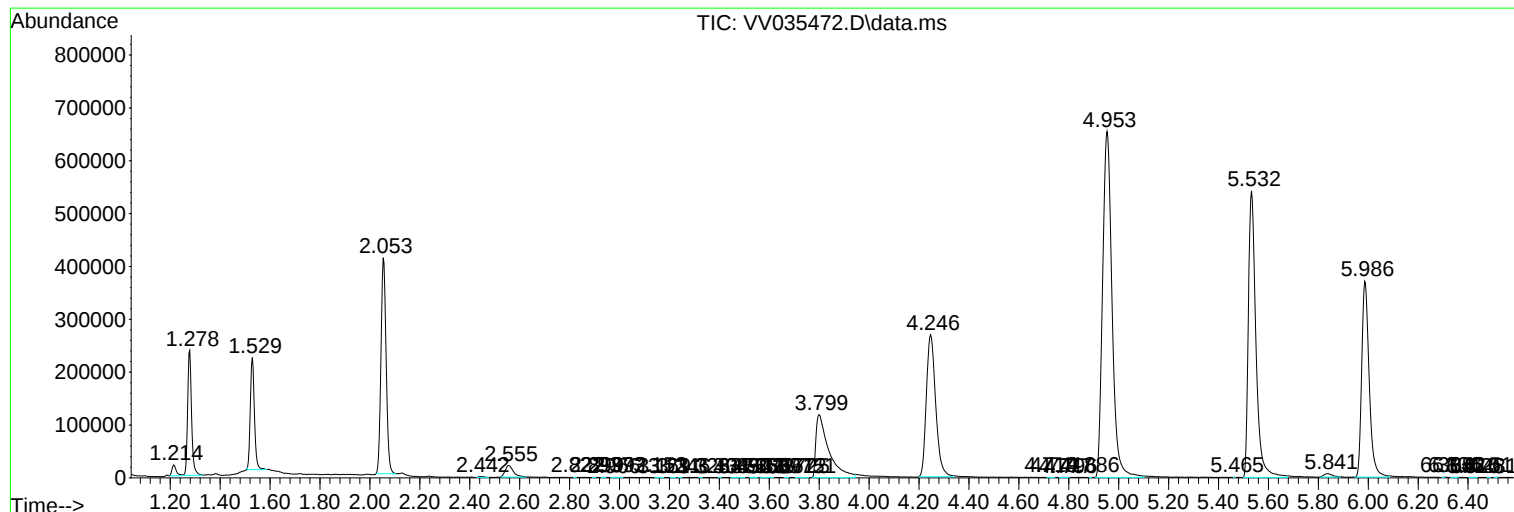

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035472.D
Acq On : 29 Apr 2024 15:45
Operator : SY/MD
Sample : P2279-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035472.D
Acq On : 29 Apr 2024 15:45
Operator : SY/MD
Sample : P2279-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------