

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035473.D
 Acq On : 29 Apr 2024 16:09
 Operator : SY/MD
 Sample : P2279-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035473.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	41	45	49	rBV	3116	3051	0.18%	0.023%
2	1.214	49	54	59	rBV	4009	4781	0.28%	0.037%
3	1.278	66	74	88	rBV	235483	253828	14.99%	1.940%
4	1.529	144	152	164	rBV	206460	239034	14.11%	1.827%
5	2.053	305	315	333	rBV	402031	582774	34.41%	4.454%
6	2.237	367	372	378	rVB4	946	1345	0.08%	0.010%
7	2.446	431	437	445	rBV4	1472	2146	0.13%	0.016%
8	2.558	460	472	496	rVV	19366	44592	2.63%	0.341%
9	2.732	525	526	531	rVB3	360	230	0.01%	0.002%
10	2.799	543	547	553	rBV3	349	304	0.02%	0.002%
11	2.841	556	560	565	rVB3	286	262	0.02%	0.002%
12	2.973	599	601	606	rVB2	292	218	0.01%	0.002%
13	3.011	607	613	616	rBV4	342	336	0.02%	0.003%
14	3.548	778	780	789	rVB2	231	277	0.02%	0.002%
15	3.712	826	831	835	rVB2	340	274	0.02%	0.002%
16	3.748	835	842	845	rBV	287	368	0.02%	0.003%
17	3.799	849	858	906	rBV	119521	410120	24.22%	3.135%
18	4.246	981	997	1031	rBV	269414	691019	40.80%	5.282%
19	4.561	1092	1095	1098	rBV2	472	407	0.02%	0.003%
20	4.725	1143	1146	1150	rVB2	513	323	0.02%	0.002%
21	4.751	1150	1154	1159	rBV3	359	383	0.02%	0.003%
22	4.789	1159	1166	1169	rBV2	341	401	0.02%	0.003%
23	4.953	1201	1217	1258	rBV2	647544	1693532	100.00%	12.944%
24	5.310	1327	1328	1333	rVB2	665	487	0.03%	0.004%
25	5.339	1334	1337	1340	rBV5	459	257	0.02%	0.002%
26	5.426	1362	1364	1367	rVB2	448	237	0.01%	0.002%
27	5.458	1367	1374	1380	rBV3	482	712	0.04%	0.005%
28	5.532	1386	1397	1438	rBV	536269	1123378	66.33%	8.586%
29	5.834	1482	1491	1508	rVB4	5834	14104	0.83%	0.108%
30	5.928	1517	1520	1523	rBV	801	502	0.03%	0.004%
31	5.986	1525	1538	1567	rBV	363192	762673	45.03%	5.829%
32	6.297	1632	1635	1642	rVB4	655	741	0.04%	0.006%
33	6.780	1781	1785	1788	rBV2	355	317	0.02%	0.002%
34	6.912	1816	1826	1852	rBV	176561	346513	20.46%	2.649%
35	7.166	1902	1905	1911	rVB3	367	390	0.02%	0.003%
36	7.243	1917	1929	1964	rBV	712385	1268841	74.92%	9.698%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035473.D
 Acq On : 29 Apr 2024 16:09
 Operator : SY/MD
 Sample : P2279-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	7.555	2015	2026	2048	rBV	122340	229537	13.55%	1.754%
38	7.809	2100	2105	2106	rBV2	447	310	0.02%	0.002%
39	7.860	2116	2121	2123	rBV3	328	320	0.02%	0.002%
40	7.873	2123	2125	2129	rVV3	449	293	0.02%	0.002%
41	7.924	2139	2141	2144	rBV2	443	218	0.01%	0.002%
42	7.986	2158	2160	2164	rVB3	594	355	0.02%	0.003%
43	8.031	2164	2174	2227	rBV3	335396	803294	47.43%	6.140%
44	8.368	2277	2279	2285	rVB3	750	539	0.03%	0.004%
45	8.484	2312	2315	2317	rVV2	399	241	0.01%	0.002%
46	8.500	2317	2320	2322	rVB3	458	267	0.02%	0.002%
47	8.580	2342	2345	2354	rVB3	811	1018	0.06%	0.008%
48	8.629	2357	2360	2363	rBV2	491	295	0.02%	0.002%
49	8.686	2375	2378	2383	rBV2	766	690	0.04%	0.005%
50	8.738	2392	2394	2397	rBV2	322	241	0.01%	0.002%
51	8.783	2397	2408	2444	rBV	822484	1373498	81.10%	10.498%
52	9.008	2476	2478	2481	rVB5	632	360	0.02%	0.003%
53	9.027	2481	2484	2490	rVB3	861	754	0.04%	0.006%
54	9.072	2495	2498	2503	rVB3	371	249	0.01%	0.002%
55	9.092	2503	2504	2507	rVB	479	239	0.01%	0.002%
56	9.114	2507	2511	2513	rBV2	458	244	0.01%	0.002%
57	9.149	2518	2522	2523	rBV	356	236	0.01%	0.002%
58	9.172	2523	2529	2535	rVB2	744	944	0.06%	0.007%
59	9.198	2535	2537	2540	rBV2	426	264	0.02%	0.002%
60	9.265	2553	2558	2559	rBV3	361	250	0.01%	0.002%
61	9.275	2559	2561	2565	rVV	325	232	0.01%	0.002%
62	9.362	2586	2588	2590	rVV	369	218	0.01%	0.002%
63	9.413	2599	2604	2608	rBV	232	301	0.02%	0.002%
64	9.551	2643	2647	2650	rBV2	330	279	0.02%	0.002%
65	9.728	2699	2702	2705	rBV2	351	239	0.01%	0.002%
66	9.998	2784	2786	2790	rVV	327	245	0.01%	0.002%
67	10.024	2790	2794	2798	rVV3	217	257	0.02%	0.002%
68	10.063	2802	2806	2811	rVB	392	314	0.02%	0.002%
69	10.149	2821	2833	2862	rBV	552044	884891	52.25%	6.764%
70	10.326	2881	2888	2894	rBV2	650	834	0.05%	0.006%
71	10.622	2974	2980	2982	rVV3	318	258	0.02%	0.002%
72	10.664	2991	2993	3001	rVB2	293	329	0.02%	0.003%
73	10.956	3078	3084	3087	rBV2	223	267	0.02%	0.002%
74	11.130	3128	3138	3144	rBV5	2943	4312	0.25%	0.033%
75	11.185	3144	3155	3182	rVV	722250	1161304	68.57%	8.876%
76	11.519	3248	3259	3260	rBV5	3045	4638	0.27%	0.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035473.D
 Acq On : 29 Apr 2024 16:09
 Operator : SY/MD
 Sample : P2279-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	11.558	3260	3271	3299	rVB	701664	1142252	67.45%	8.731%
78	11.792	3342	3344	3349	rVB4	744	450	0.03%	0.003%
79	11.879	3368	3371	3373	rBV	703	417	0.02%	0.003%
80	11.911	3378	3381	3384	rBV3	364	256	0.02%	0.002%
81	11.976	3397	3401	3406	rVB3	483	396	0.02%	0.003%
82	12.024	3412	3416	3417	rBV2	356	229	0.01%	0.002%
83	12.114	3441	3444	3449	rVB5	514	390	0.02%	0.003%
84	12.194	3466	3469	3472	rVV2	653	486	0.03%	0.004%
85	12.246	3482	3485	3488	rVB2	452	266	0.02%	0.002%
86	12.294	3496	3500	3504	rBV3	424	416	0.02%	0.003%
87	12.323	3504	3509	3513	rVV2	230	256	0.02%	0.002%
88	12.641	3603	3608	3610	rBV2	494	463	0.03%	0.004%
89	12.712	3626	3630	3635	rBV2	424	353	0.02%	0.003%
90	12.770	3646	3648	3653	rVB2	567	404	0.02%	0.003%
91	12.857	3670	3675	3678	rBV3	326	337	0.02%	0.003%
92	13.207	3777	3784	3792	rBV6	5615	8308	0.49%	0.064%
93	13.503	3872	3876	3879	rVB4	589	427	0.03%	0.003%
94	13.522	3880	3882	3886	rBV	363	232	0.01%	0.002%
95	13.577	3897	3899	3902	rBV	455	277	0.02%	0.002%
96	13.689	3927	3934	3937	rBV5	1976	2133	0.13%	0.016%
97	13.847	3980	3983	3986	rBV2	418	274	0.02%	0.002%
98	14.455	4169	4172	4178	rBV3	513	582	0.03%	0.004%
99	14.667	4235	4238	4242	rBV3	464	413	0.02%	0.003%
100	14.869	4299	4301	4304	rBV3	664	432	0.03%	0.003%




Sum of corrected areas: 13083180

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035473.D
Acq On : 29 Apr 2024 16:09
Operator : SY/MD
Sample : P2279-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

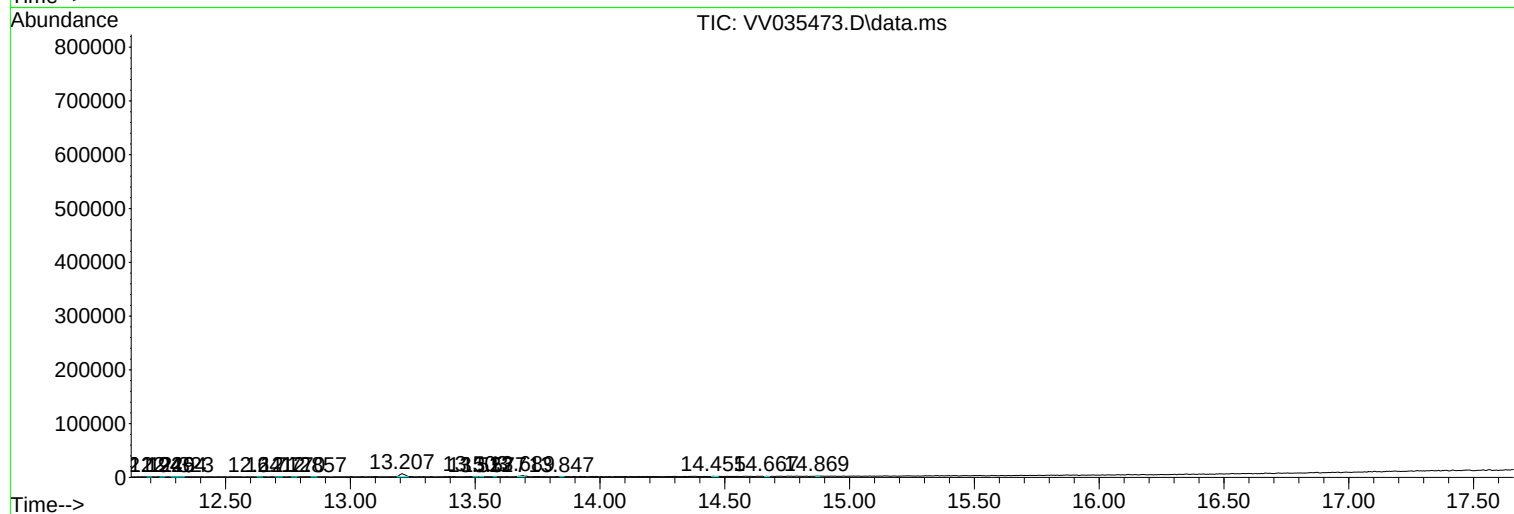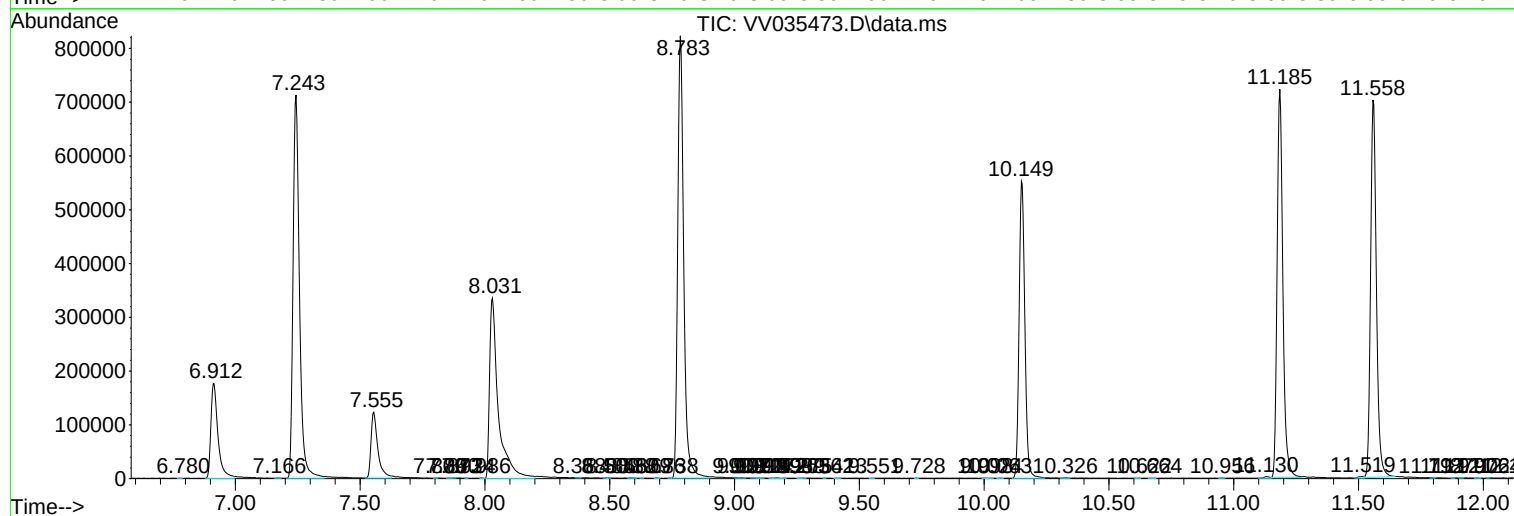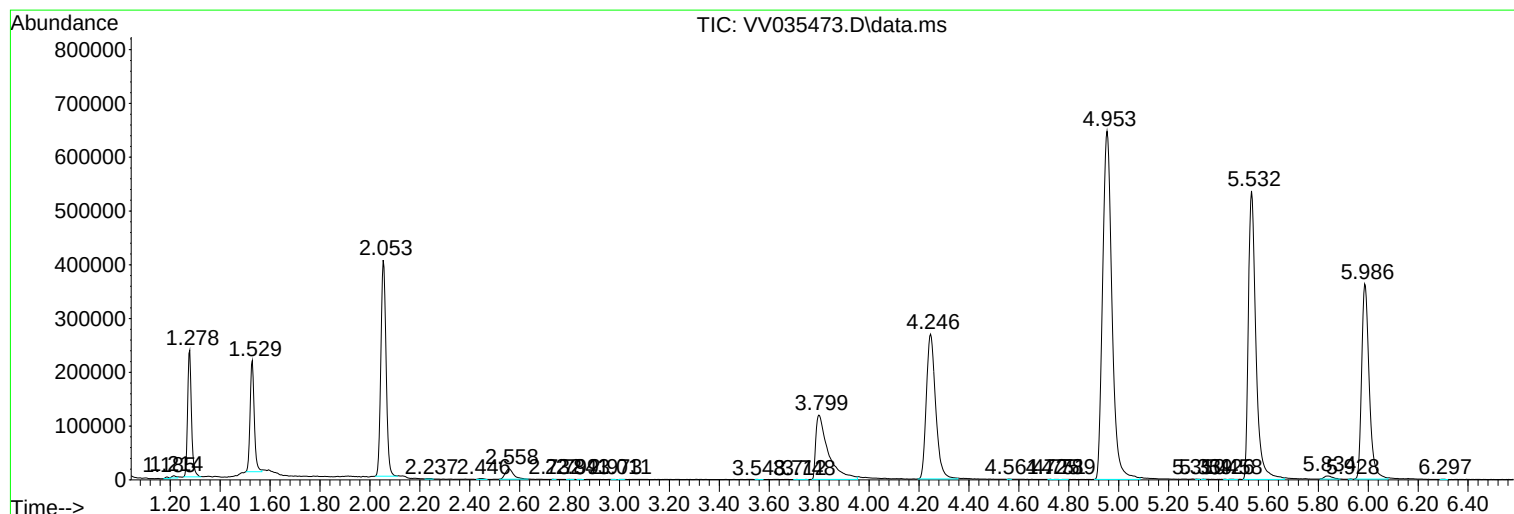

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035473.D
Acq On : 29 Apr 2024 16:09
Operator : SY/MD
Sample : P2279-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035473.D
Acq On : 29 Apr 2024 16:09
Operator : SY/MD
Sample : P2279-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------