

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035474.D
 Acq On : 29 Apr 2024 16:33
 Operator : SY/MD
 Sample : P2279-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035474.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.185	41	45	48	rBV	2849	2395	0.13%	0.017%
2	1.214	48	54	64	rVV	20348	24850	1.38%	0.177%
3	1.278	66	74	91	rVB	243824	269238	14.97%	1.917%
4	1.529	145	152	164	rBV	203958	234595	13.05%	1.670%
5	2.053	305	315	334	rBV	421523	609633	33.91%	4.340%
6	2.236	364	372	380	rVB3	1584	2490	0.14%	0.018%
7	2.307	392	394	397	rVB2	719	372	0.02%	0.003%
8	2.359	408	410	412	rBV2	523	277	0.02%	0.002%
9	2.397	419	422	423	rBV	341	221	0.01%	0.002%
10	2.449	431	438	450	rVB5	2423	4359	0.24%	0.031%
11	2.497	450	453	456	rBV2	353	295	0.02%	0.002%
12	2.558	459	472	487	rBV	15405	38213	2.13%	0.272%
13	2.696	509	515	517	rBV5	1432	1461	0.08%	0.010%
14	3.108	638	643	646	rBV3	776	657	0.04%	0.005%
15	3.249	683	687	690	rBV	284	175	0.01%	0.001%
16	3.278	690	696	700	rBV2	167	237	0.01%	0.002%
17	3.664	807	816	820	rBV3	536	510	0.03%	0.004%
18	3.757	843	845	849	rBV2	262	216	0.01%	0.002%
19	3.802	849	859	918	rBV	127915	457371	25.44%	3.256%
20	4.246	980	997	1026	rBV	286346	736457	40.96%	5.243%
21	4.416	1048	1050	1055	rVB2	688	573	0.03%	0.004%
22	4.442	1055	1058	1060	rBV	444	219	0.01%	0.002%
23	4.648	1120	1122	1126	rVB3	396	240	0.01%	0.002%
24	4.735	1142	1149	1151	rBV5	1093	1227	0.07%	0.009%
25	4.953	1201	1217	1264	rBV2	679369	1797980	100.00%	12.800%
26	5.281	1317	1319	1324	rVB2	647	384	0.02%	0.003%
27	5.330	1329	1334	1335	rBV3	434	280	0.02%	0.002%
28	5.532	1385	1397	1434	rBV	577392	1211356	67.37%	8.624%
29	5.764	1467	1469	1476	rBV5	777	651	0.04%	0.005%
30	5.834	1483	1491	1511	rVB7	7681	18467	1.03%	0.131%
31	5.912	1512	1515	1516	rBV2	568	209	0.01%	0.001%
32	5.931	1519	1521	1522	rBV	491	262	0.01%	0.002%
33	5.986	1526	1538	1570	rBV	386053	812232	45.17%	5.782%
34	6.220	1610	1611	1614	rVB	354	173	0.01%	0.001%
35	6.304	1633	1637	1643	rVB4	499	457	0.03%	0.003%
36	6.371	1655	1658	1663	rVB3	354	294	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035474.D
 Acq On : 29 Apr 2024 16:33
 Operator : SY/MD
 Sample : P2279-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.416	1670	1672	1674	rVB	434	189	0.01%	0.001%
38	6.439	1674	1679	1682	rBV2	677	694	0.04%	0.005%
39	6.519	1702	1704	1710	rVB2	305	238	0.01%	0.002%
40	6.593	1718	1727	1731	rBV2	354	438	0.02%	0.003%
41	6.670	1749	1751	1755	rVB2	250	191	0.01%	0.001%
42	6.715	1763	1765	1768	rVB2	378	219	0.01%	0.002%
43	6.738	1768	1772	1775	rBV4	525	435	0.02%	0.003%
44	6.912	1816	1826	1855	rBV	190309	372259	20.70%	2.650%
45	7.140	1895	1897	1903	rBV3	425	489	0.03%	0.003%
46	7.166	1903	1905	1907	rBV	313	186	0.01%	0.001%
47	7.243	1917	1929	1962	rBV	754812	1351954	75.19%	9.624%
48	7.555	2017	2026	2060	rBV	132478	250430	13.93%	1.783%
49	7.796	2097	2101	2103	rBV3	661	583	0.03%	0.004%
50	7.860	2119	2121	2125	rVB3	421	276	0.02%	0.002%
51	7.912	2132	2137	2146	rVB5	1302	1686	0.09%	0.012%
52	7.985	2155	2160	2164	rBV4	486	387	0.02%	0.003%
53	8.030	2164	2174	2219	rBV2	380679	887568	49.36%	6.319%
54	8.468	2305	2310	2313	rVB3	563	519	0.03%	0.004%
55	8.487	2313	2316	2320	rBV3	465	343	0.02%	0.002%
56	8.513	2323	2324	2330	rVB3	529	355	0.02%	0.003%
57	8.783	2397	2408	2450	rVV	898225	1486645	82.68%	10.583%
58	9.088	2501	2503	2505	rBV3	888	522	0.03%	0.004%
59	9.153	2520	2523	2525	rVB2	341	187	0.01%	0.001%
60	9.172	2525	2529	2534	rBV3	359	300	0.02%	0.002%
61	9.194	2534	2536	2538	rVV3	539	252	0.01%	0.002%
62	9.214	2540	2542	2548	rVB	443	433	0.02%	0.003%
63	9.272	2556	2560	2562	rBV2	537	348	0.02%	0.002%
64	9.284	2562	2564	2570	rVB2	660	528	0.03%	0.004%
65	9.500	2626	2631	2634	rBV2	838	799	0.04%	0.006%
66	9.674	2679	2685	2695	rBV4	474	680	0.04%	0.005%
67	9.770	2711	2715	2717	rBV	355	233	0.01%	0.002%
68	9.828	2730	2733	2738	rVB3	320	262	0.01%	0.002%
69	9.876	2743	2748	2754	rBV2	1151	1275	0.07%	0.009%
70	9.928	2761	2764	2767	rVB3	267	180	0.01%	0.001%
71	9.979	2777	2780	2784	rBV2	441	351	0.02%	0.002%
72	10.072	2806	2809	2813	rBV	270	222	0.01%	0.002%
73	10.153	2820	2834	2864	rBV	600627	971228	54.02%	6.914%
74	10.323	2882	2887	2893	rBV4	430	505	0.03%	0.004%
75	10.394	2905	2909	2914	rBV2	313	367	0.02%	0.003%
76	10.487	2933	2938	2944	rBV3	796	1092	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035474.D
 Acq On : 29 Apr 2024 16:33
 Operator : SY/MD
 Sample : P2279-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	10.603	2971	2974	2977	rVB2	312	194	0.01%	0.001%
78	10.693	3000	3002	3005	rVB2	379	187	0.01%	0.001%
79	10.786	3029	3031	3036	rVB4	520	308	0.02%	0.002%
80	10.860	3050	3054	3056	rBV3	622	544	0.03%	0.004%
81	10.915	3066	3071	3073	rBV	301	252	0.01%	0.002%
82	11.056	3111	3115	3119	rBV2	222	196	0.01%	0.001%
83	11.130	3132	3138	3144	rBV4	3144	4783	0.27%	0.034%
84	11.185	3144	3155	3179	rBV	807825	1251389	69.60%	8.909%
85	11.461	3238	3241	3247	rVB4	451	385	0.02%	0.003%
86	11.509	3247	3256	3260	rBV5	4752	8461	0.47%	0.060%
87	11.558	3261	3271	3308	rVB	758134	1205427	67.04%	8.581%
88	12.079	3430	3433	3435	rBV3	325	257	0.01%	0.002%
89	12.300	3500	3502	3505	rVV2	328	192	0.01%	0.001%
90	12.371	3521	3524	3528	rBV2	600	351	0.02%	0.002%
91	12.448	3545	3548	3551	rBV2	404	271	0.02%	0.002%
92	12.583	3587	3590	3593	rVV3	700	562	0.03%	0.004%
93	12.722	3631	3633	3637	rVV4	353	226	0.01%	0.002%
94	12.744	3637	3640	3644	rVV3	402	314	0.02%	0.002%
95	12.796	3653	3656	3660	rVB3	476	360	0.02%	0.003%
96	13.214	3779	3786	3797	rVV7	2565	4286	0.24%	0.031%
97	13.316	3815	3818	3819	rBV	291	198	0.01%	0.001%
98	13.387	3838	3840	3844	rBV2	349	201	0.01%	0.001%
99	13.542	3886	3888	3891	rBV4	328	220	0.01%	0.002%
100	13.689	3927	3934	3943	rBV7	1582	2587	0.14%	0.018%




Sum of corrected areas: 14047025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035474.D
Acq On : 29 Apr 2024 16:33
Operator : SY/MD
Sample : P2279-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

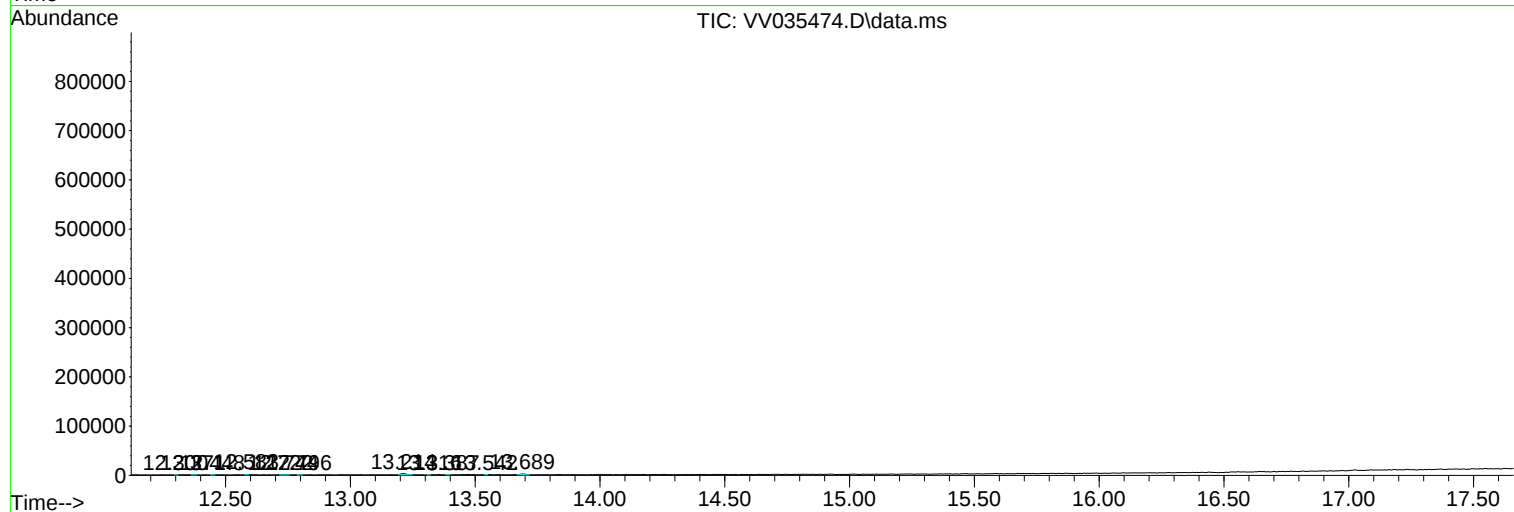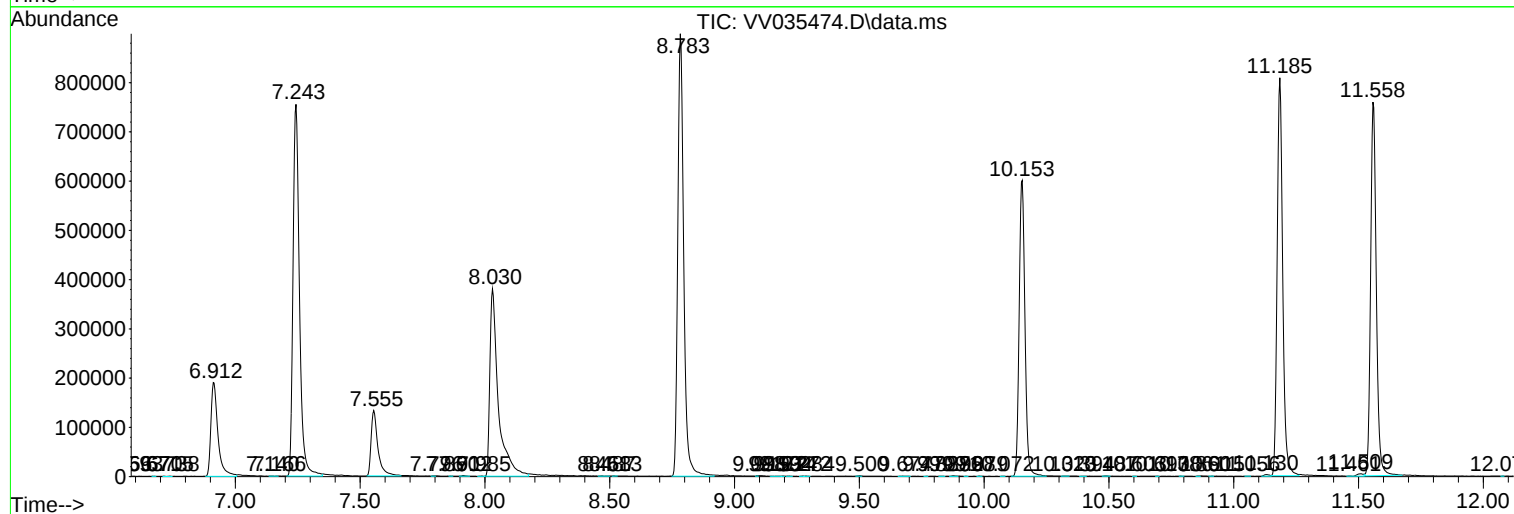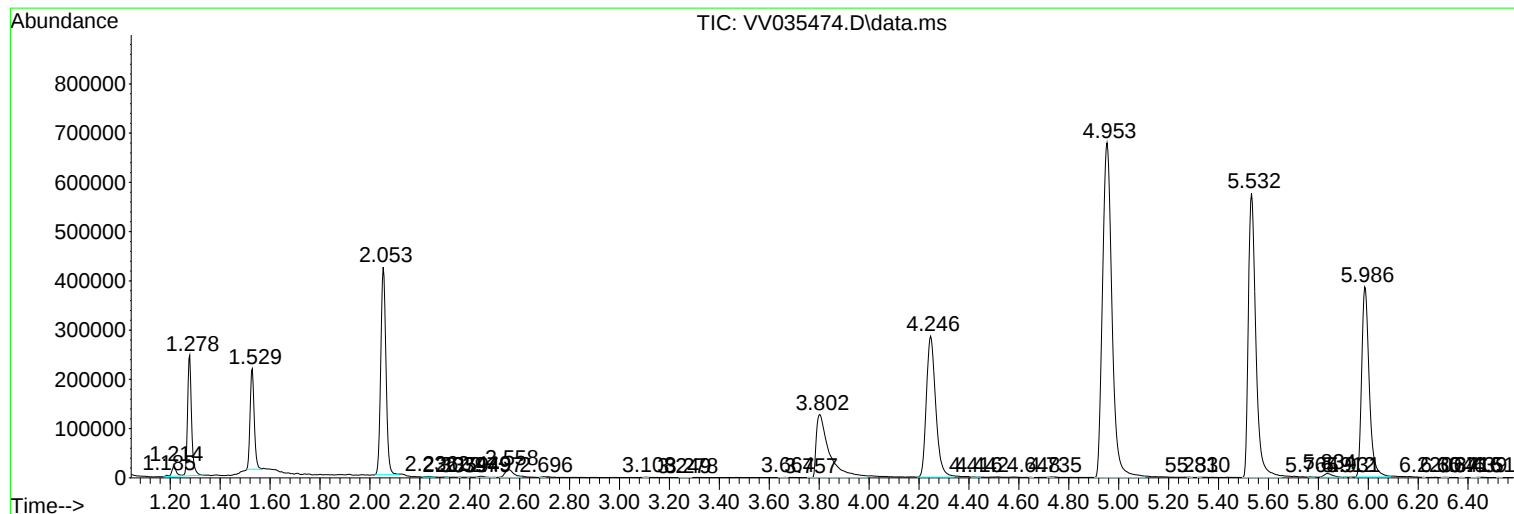

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035474.D
Acq On : 29 Apr 2024 16:33
Operator : SY/MD
Sample : P2279-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035474.D
Acq On : 29 Apr 2024 16:33
Operator : SY/MD
Sample : P2279-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------