

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035475.D
 Acq On : 29 Apr 2024 16:57
 Operator : SY/MD
 Sample : P2279-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	42	46	49	rBV2	1947	1713	0.11%	0.014%
2	1.214	49	54	59	rBV2	5557	6084	0.39%	0.051%
3	1.278	67	74	92	rVB	211566	229526	14.88%	1.929%
4	1.529	145	152	165	rBV	190146	216630	14.04%	1.821%
5	2.056	306	316	331	rBV	361594	523458	33.93%	4.399%
6	2.236	364	372	384	rVB7	2083	3912	0.25%	0.033%
7	2.346	404	406	411	rVB2	746	413	0.03%	0.003%
8	2.378	411	416	419	rBV4	637	763	0.05%	0.006%
9	2.439	432	435	436	rBV2	530	331	0.02%	0.003%
10	2.555	458	471	493	rBV	6824	16045	1.04%	0.135%
11	2.674	504	508	513	rVB3	450	393	0.03%	0.003%
12	2.741	525	529	532	rVB	343	238	0.02%	0.002%
13	2.812	546	551	554	rVB2	256	245	0.02%	0.002%
14	2.879	566	572	574	rBV3	503	401	0.03%	0.003%
15	2.963	597	598	607	rVB2	413	348	0.02%	0.003%
16	3.413	734	738	741	rBV	394	228	0.01%	0.002%
17	3.683	816	822	826	rVB2	296	329	0.02%	0.003%
18	3.799	849	858	894	rBV	109436	354854	23.00%	2.982%
19	4.178	974	976	978	rBV2	463	305	0.02%	0.003%
20	4.246	981	997	1038	rVV	244738	635153	41.17%	5.338%
21	4.571	1091	1098	1102	rBV5	343	431	0.03%	0.004%
22	4.603	1104	1108	1111	rVB3	377	273	0.02%	0.002%
23	4.719	1137	1144	1146	rBV3	521	476	0.03%	0.004%
24	4.776	1160	1162	1167	rBV2	400	341	0.02%	0.003%
25	4.953	1201	1217	1258	rBV2	588235	1542570	100.00%	12.964%
26	5.288	1319	1321	1324	rVV2	593	280	0.02%	0.002%
27	5.532	1386	1397	1440	rBV	430481	919868	59.63%	7.731%
28	5.834	1482	1491	1493	rBV4	5823	6989	0.45%	0.059%
29	5.989	1526	1539	1568	rBV	330680	695895	45.11%	5.848%
30	6.223	1608	1612	1614	rVB3	441	335	0.02%	0.003%
31	6.246	1616	1619	1623	rVV4	393	284	0.02%	0.002%
32	6.329	1640	1645	1646	rBV	290	235	0.02%	0.002%
33	6.529	1703	1707	1712	rBV2	281	310	0.02%	0.003%
34	6.596	1725	1728	1730	rBV2	460	321	0.02%	0.003%
35	6.657	1740	1747	1750	rBV2	270	312	0.02%	0.003%
36	6.915	1816	1827	1858	rBV	158602	315095	20.43%	2.648%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035475.D
 Acq On : 29 Apr 2024 16:57
 Operator : SY/MD
 Sample : P2279-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	7.243	1918	1929	1957	rBV	632130	1137387	73.73%	9.559%
38	7.506	2008	2011	2014	rBB3	489	283	0.02%	0.002%
39	7.555	2015	2026	2063	rBV	109324	214341	13.90%	1.801%
40	7.767	2088	2092	2097	rBV2	811	582	0.04%	0.005%
41	7.789	2097	2099	2102	rVB2	510	268	0.02%	0.002%
42	7.815	2105	2107	2111	rVB2	440	274	0.02%	0.002%
43	7.847	2114	2117	2122	rBV2	524	459	0.03%	0.004%
44	7.889	2127	2130	2135	rVB3	549	428	0.03%	0.004%
45	7.915	2135	2138	2139	rBV2	456	233	0.02%	0.002%
46	8.030	2164	2174	2215	rBV2	308847	731698	47.43%	6.149%
47	8.381	2281	2283	2286	rVB2	885	444	0.03%	0.004%
48	8.400	2286	2289	2292	rVB4	391	259	0.02%	0.002%
49	8.423	2292	2296	2299	rVB2	570	453	0.03%	0.004%
50	8.519	2322	2326	2330	rVB3	689	615	0.04%	0.005%
51	8.564	2334	2340	2342	rBV3	579	479	0.03%	0.004%
52	8.622	2356	2358	2363	rVB2	467	278	0.02%	0.002%
53	8.722	2383	2389	2392	rVB4	627	604	0.04%	0.005%
54	8.744	2393	2396	2397	rBV	530	255	0.02%	0.002%
55	8.783	2397	2408	2449	rVV	680189	1284002	83.24%	10.791%
56	8.998	2471	2475	2477	rVV3	751	479	0.03%	0.004%
57	9.011	2477	2479	2484	rVB2	398	297	0.02%	0.002%
58	9.050	2489	2491	2496	rVB3	431	247	0.02%	0.002%
59	9.079	2496	2500	2505	rBV4	346	367	0.02%	0.003%
60	9.104	2505	2508	2511	rVB3	380	253	0.02%	0.002%
61	9.127	2512	2515	2521	rVB3	466	397	0.03%	0.003%
62	9.172	2526	2529	2535	rBV5	372	375	0.02%	0.003%
63	9.468	2616	2621	2625	rBV2	388	389	0.03%	0.003%
64	9.731	2700	2703	2710	rVB2	329	277	0.02%	0.002%
65	9.789	2716	2721	2724	rBV3	332	318	0.02%	0.003%
66	10.152	2821	2834	2865	rBV	510288	816977	52.96%	6.866%
67	10.310	2879	2883	2884	rBV2	370	229	0.01%	0.002%
68	10.333	2887	2890	2895	rVV2	813	631	0.04%	0.005%
69	10.423	2914	2918	2922	rBV2	473	293	0.02%	0.002%
70	10.548	2951	2957	2959	rBV2	266	276	0.02%	0.002%
71	10.693	2999	3002	3004	rBV	525	268	0.02%	0.002%
72	10.837	3042	3047	3051	rBV2	269	308	0.02%	0.003%
73	11.123	3127	3136	3145	rBV	21676	35693	2.31%	0.300%
74	11.185	3145	3155	3191	rVB2	607771	1106668	71.74%	9.301%
75	11.416	3224	3227	3230	rBV4	361	255	0.02%	0.002%
76	11.561	3259	3272	3300	rBV	634242	1075521	69.72%	9.039%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035475.D
 Acq On : 29 Apr 2024 16:57
 Operator : SY/MD
 Sample : P2279-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	11.744	3327	3329	3332	rVB2	813	463	0.03%	0.004%
78	11.953	3390	3394	3395	rBV2	507	296	0.02%	0.002%
79	12.156	3454	3457	3461	rVB3	438	286	0.02%	0.002%
80	12.194	3466	3469	3470	rBV	412	282	0.02%	0.002%
81	12.281	3492	3496	3498	rVB2	447	266	0.02%	0.002%
82	12.345	3513	3516	3519	rBV4	355	265	0.02%	0.002%
83	12.458	3547	3551	3554	rBV2	417	348	0.02%	0.003%
84	12.500	3562	3564	3568	rVB2	414	234	0.02%	0.002%
85	12.641	3605	3608	3611	rBV2	318	260	0.02%	0.002%
86	12.783	3646	3652	3658	rBV5	411	689	0.04%	0.006%
87	12.937	3695	3700	3702	rBV	386	377	0.02%	0.003%
88	13.165	3766	3771	3772	rBV	353	251	0.02%	0.002%
89	13.213	3778	3786	3792	rBV6	901	1573	0.10%	0.013%
90	13.377	3834	3837	3839	rBV2	454	234	0.02%	0.002%
91	13.522	3879	3882	3886	rBV2	598	445	0.03%	0.004%
92	13.541	3886	3888	3891	rBV2	337	233	0.02%	0.002%
93	13.641	3915	3919	3923	rBV2	476	401	0.03%	0.003%
94	13.853	3983	3985	3989	rVB2	489	239	0.02%	0.002%
95	14.127	4067	4070	4075	rVB2	649	490	0.03%	0.004%
96	14.480	4177	4180	4187	rVB4	791	837	0.05%	0.007%
97	14.516	4188	4191	4194	rBV3	421	349	0.02%	0.003%
98	14.535	4195	4197	4199	rBV2	437	241	0.02%	0.002%
99	14.551	4199	4202	4205	rBV3	506	420	0.03%	0.004%
100	14.602	4216	4218	4221	rVB	490	231	0.01%	0.002%




Sum of corrected areas: 11898954

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035475.D
Acq On : 29 Apr 2024 16:57
Operator : SY/MD
Sample : P2279-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

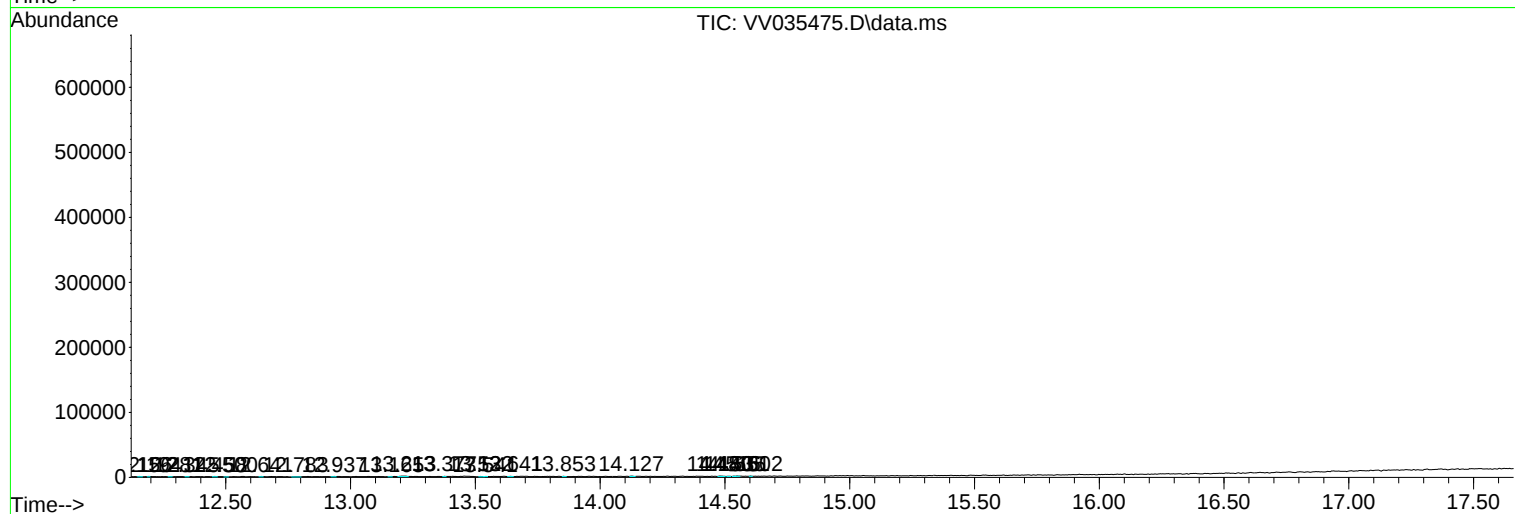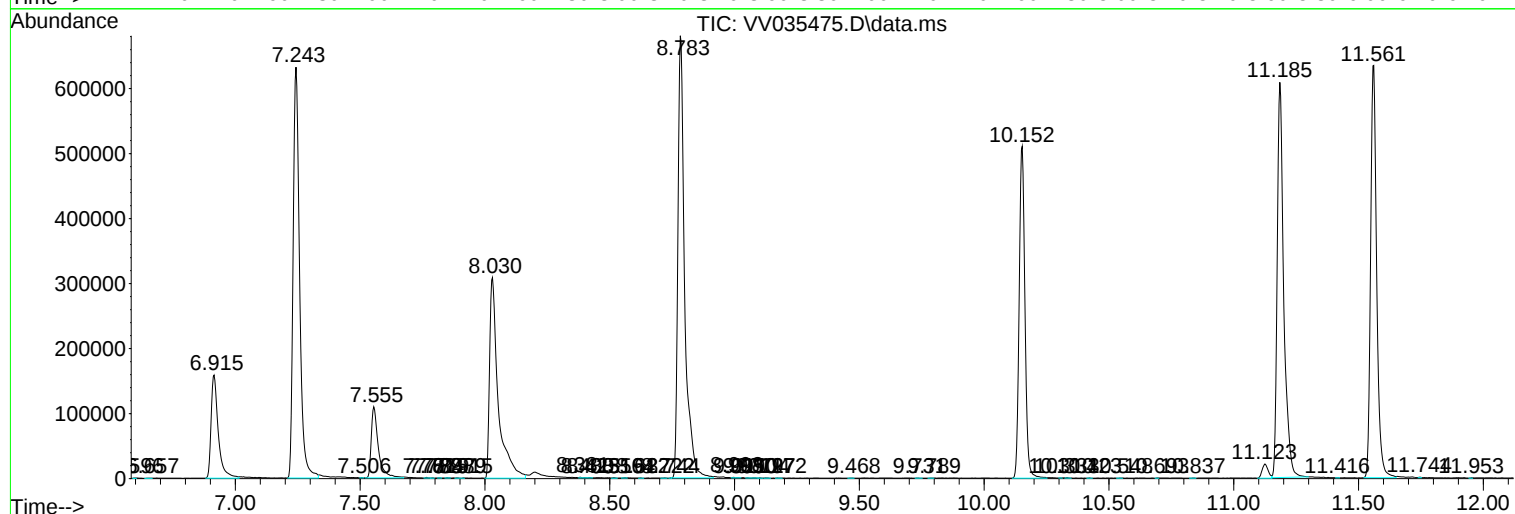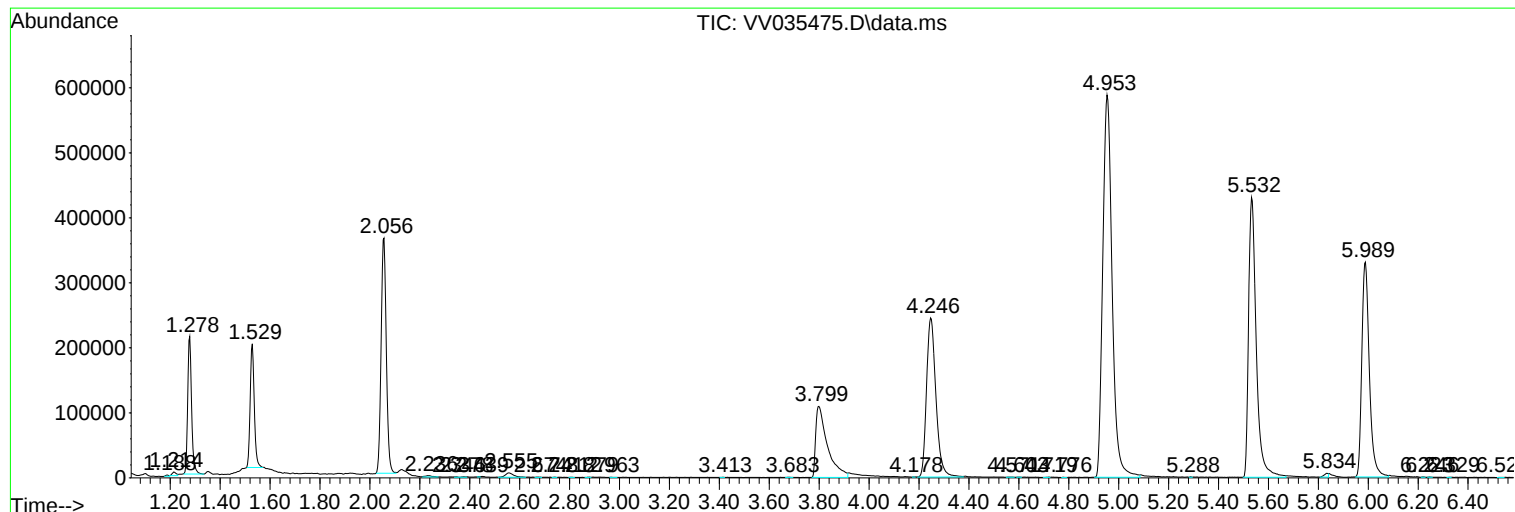

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035475.D
Acq On : 29 Apr 2024 16:57
Operator : SY/MD
Sample : P2279-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035475.D
Acq On : 29 Apr 2024 16:57
Operator : SY/MD
Sample : P2279-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc