

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035476.D
 Acq On : 29 Apr 2024 17:21
 Operator : SY/MD
 Sample : P2279-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	42	46	48	rBV2	1875	1425	0.12%	0.015%
2	1.214	49	54	64	rVV	12534	15754	1.29%	0.165%
3	1.278	67	74	88	rVB	171460	188658	15.40%	1.971%
4	1.529	145	152	168	rBV	152561	175072	14.29%	1.829%
5	2.053	305	315	331	rBV	290222	423121	34.54%	4.420%
6	2.297	389	391	394	rBV3	443	277	0.02%	0.003%
7	2.439	428	435	436	rBV3	914	756	0.06%	0.008%
8	2.558	455	472	489	rBV	21295	49248	4.02%	0.515%
9	2.731	522	526	529	rBV2	337	283	0.02%	0.003%
10	3.088	634	637	642	rBV	213	223	0.02%	0.002%
11	3.220	676	678	683	rVB2	399	273	0.02%	0.003%
12	3.407	732	736	739	rBV2	310	255	0.02%	0.003%
13	3.529	771	774	782	rVB2	212	242	0.02%	0.003%
14	3.603	793	797	800	rVB	224	199	0.02%	0.002%
15	3.632	800	806	809	rBV	197	222	0.02%	0.002%
16	3.802	847	859	903	rBV2	89986	331507	27.07%	3.463%
17	4.246	981	997	1035	rBV	194580	505389	41.26%	5.280%
18	4.471	1065	1067	1071	rVB3	393	220	0.02%	0.002%
19	4.622	1110	1114	1124	rVB4	552	773	0.06%	0.008%
20	4.686	1130	1134	1141	rBV2	475	473	0.04%	0.005%
21	4.815	1168	1174	1176	rBV2	293	304	0.02%	0.003%
22	4.831	1176	1179	1181	rBV2	345	236	0.02%	0.002%
23	4.895	1196	1199	1202	rBV2	305	269	0.02%	0.003%
24	4.953	1202	1217	1252	rBV2	464581	1224844	100.00%	12.796%
25	5.175	1284	1286	1289	rBV2	553	334	0.03%	0.003%
26	5.407	1356	1358	1363	rVB3	317	281	0.02%	0.003%
27	5.439	1363	1368	1370	rBV	385	362	0.03%	0.004%
28	5.532	1387	1397	1440	rBV	393165	837901	68.41%	8.754%
29	5.837	1482	1492	1508	rBV4	4961	11848	0.97%	0.124%
30	5.989	1526	1539	1565	rBV	265390	557547	45.52%	5.825%
31	6.159	1588	1592	1595	rBV4	807	701	0.06%	0.007%
32	6.210	1606	1608	1611	rVB2	519	284	0.02%	0.003%
33	6.262	1622	1624	1630	rVB2	450	408	0.03%	0.004%
34	6.381	1656	1661	1664	rBV2	333	312	0.03%	0.003%
35	6.407	1668	1669	1676	rVB2	349	249	0.02%	0.003%
36	6.445	1676	1681	1684	rBV	383	352	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035476.D
 Acq On : 29 Apr 2024 17:21
 Operator : SY/MD
 Sample : P2279-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.464	1684	1687	1694	rVB2	335	291	0.02%	0.003%
38	6.783	1782	1786	1789	rBV2	282	275	0.02%	0.003%
39	6.915	1817	1827	1851	rBV	122867	244119	19.93%	2.550%
40	7.243	1918	1929	1964	rBV	494875	896187	73.17%	9.363%
41	7.558	2017	2027	2051	rBV	82476	163325	13.33%	1.706%
42	7.706	2070	2073	2077	rVB2	939	663	0.05%	0.007%
43	7.815	2105	2107	2112	rVB2	300	214	0.02%	0.002%
44	7.966	2152	2154	2160	rVB2	340	273	0.02%	0.003%
45	8.030	2165	2174	2219	rBV2	226021	564989	46.13%	5.903%
46	8.403	2286	2290	2291	rBV	417	236	0.02%	0.002%
47	8.593	2343	2349	2353	rVV4	349	331	0.03%	0.003%
48	8.667	2369	2372	2375	rBV3	238	212	0.02%	0.002%
49	8.744	2391	2396	2397	rBV	368	252	0.02%	0.003%
50	8.783	2397	2408	2437	rBV	601560	1027019	83.85%	10.729%
51	9.050	2489	2491	2492	rBV	582	322	0.03%	0.003%
52	9.123	2511	2514	2518	rVB3	694	543	0.04%	0.006%
53	9.185	2530	2533	2534	rBV2	385	226	0.02%	0.002%
54	9.230	2542	2547	2552	rBV3	285	369	0.03%	0.004%
55	9.255	2552	2555	2558	rVB	425	281	0.02%	0.003%
56	9.374	2587	2592	2593	rBV2	279	202	0.02%	0.002%
57	9.416	2601	2605	2608	rVB	340	207	0.02%	0.002%
58	9.455	2612	2617	2620	rBV2	309	340	0.03%	0.004%
59	9.474	2620	2623	2625	rVV2	392	249	0.02%	0.003%
60	9.506	2631	2633	2638	rVB	384	261	0.02%	0.003%
61	9.570	2648	2653	2654	rBV3	354	269	0.02%	0.003%
62	9.580	2654	2656	2659	rVB3	475	211	0.02%	0.002%
63	9.609	2659	2665	2669	rBV2	339	408	0.03%	0.004%
64	9.789	2718	2721	2727	rBV3	313	336	0.03%	0.004%
65	9.995	2781	2785	2788	rBV2	333	229	0.02%	0.002%
66	10.049	2799	2802	2805	rBV2	414	336	0.03%	0.004%
67	10.152	2819	2834	2861	rBV	412014	651736	53.21%	6.809%
68	10.525	2943	2950	2955	rVB3	511	571	0.05%	0.006%
69	10.551	2955	2958	2961	rBV	318	265	0.02%	0.003%
70	10.895	3060	3065	3069	rVV2	211	202	0.02%	0.002%
71	10.927	3073	3075	3078	rBV	276	201	0.02%	0.002%
72	11.130	3135	3138	3140	rBV	389	254	0.02%	0.003%
73	11.184	3145	3155	3181	rBV	535871	856264	69.91%	8.946%
74	11.500	3245	3253	3261	rBV6	7119	14346	1.17%	0.150%
75	11.561	3261	3272	3301	rVB	489532	804280	65.66%	8.402%
76	11.847	3357	3361	3365	rBV4	376	350	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035476.D
 Acq On : 29 Apr 2024 17:21
 Operator : SY/MD
 Sample : P2279-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	11.898	3375	3377	3379	rBV	435	232	0.02%	0.002%
78	12.043	3420	3422	3429	rVB4	408	380	0.03%	0.004%
79	12.156	3453	3457	3461	rVB3	518	428	0.03%	0.004%
80	12.184	3461	3466	3468	rBV3	459	387	0.03%	0.004%
81	12.271	3490	3493	3497	rVB3	490	401	0.03%	0.004%
82	12.307	3502	3504	3507	rBV3	357	210	0.02%	0.002%
83	12.329	3509	3511	3516	rVB3	483	358	0.03%	0.004%
84	12.384	3524	3528	3532	rBV3	265	274	0.02%	0.003%
85	12.419	3536	3539	3545	rVB	297	259	0.02%	0.003%
86	12.516	3566	3569	3573	rBV3	235	221	0.02%	0.002%
87	12.538	3573	3576	3580	rVB3	318	242	0.02%	0.003%
88	12.586	3588	3591	3593	rBV2	376	219	0.02%	0.002%
89	12.670	3613	3617	3622	rBV3	353	364	0.03%	0.004%
90	12.754	3640	3643	3644	rBV	482	266	0.02%	0.003%
91	12.802	3655	3658	3662	rBV3	407	378	0.03%	0.004%
92	12.905	3688	3690	3695	rBV2	299	309	0.03%	0.003%
93	13.210	3782	3785	3795	rVB3	1420	1852	0.15%	0.019%
94	13.252	3795	3798	3800	rBV2	527	335	0.03%	0.003%
95	13.278	3803	3806	3809	rBV	436	337	0.03%	0.004%
96	13.548	3884	3890	3893	rBV4	522	584	0.05%	0.006%
97	13.618	3908	3912	3914	rBV	363	287	0.02%	0.003%
98	13.692	3931	3935	3939	rVB5	687	633	0.05%	0.007%
99	13.927	4004	4008	4011	rBV3	401	360	0.03%	0.004%
100	14.191	4087	4090	4094	rVB2	569	367	0.03%	0.004%




Sum of corrected areas: 9571929

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035476.D
Acq On : 29 Apr 2024 17:21
Operator : SY/MD
Sample : P2279-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

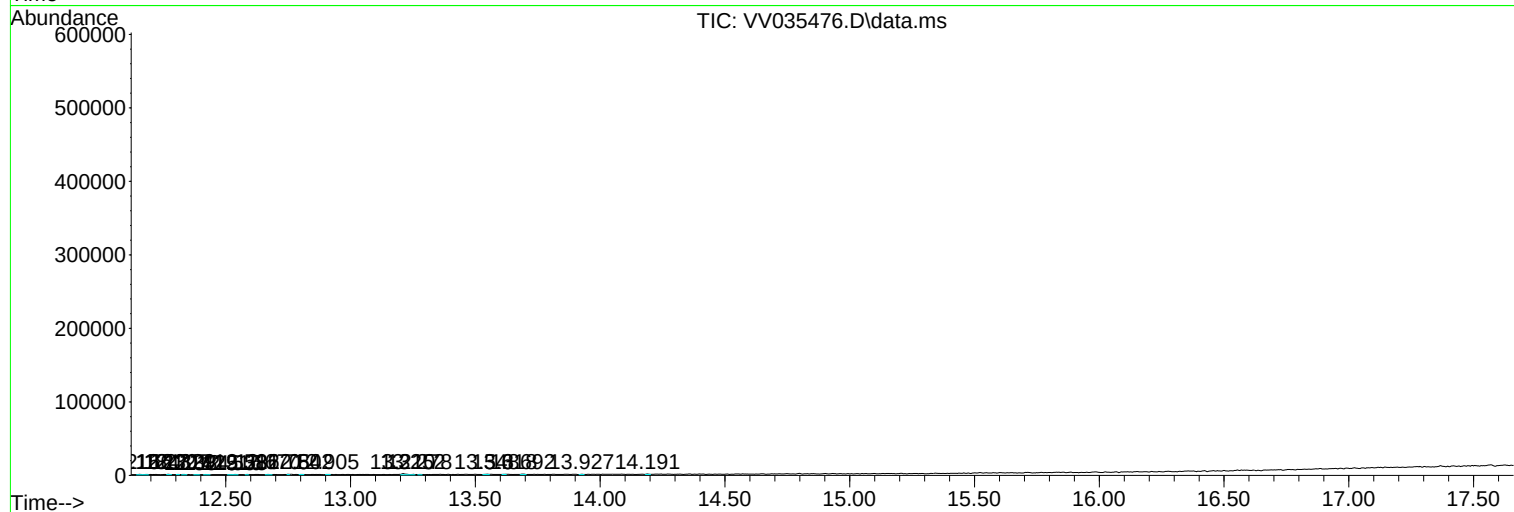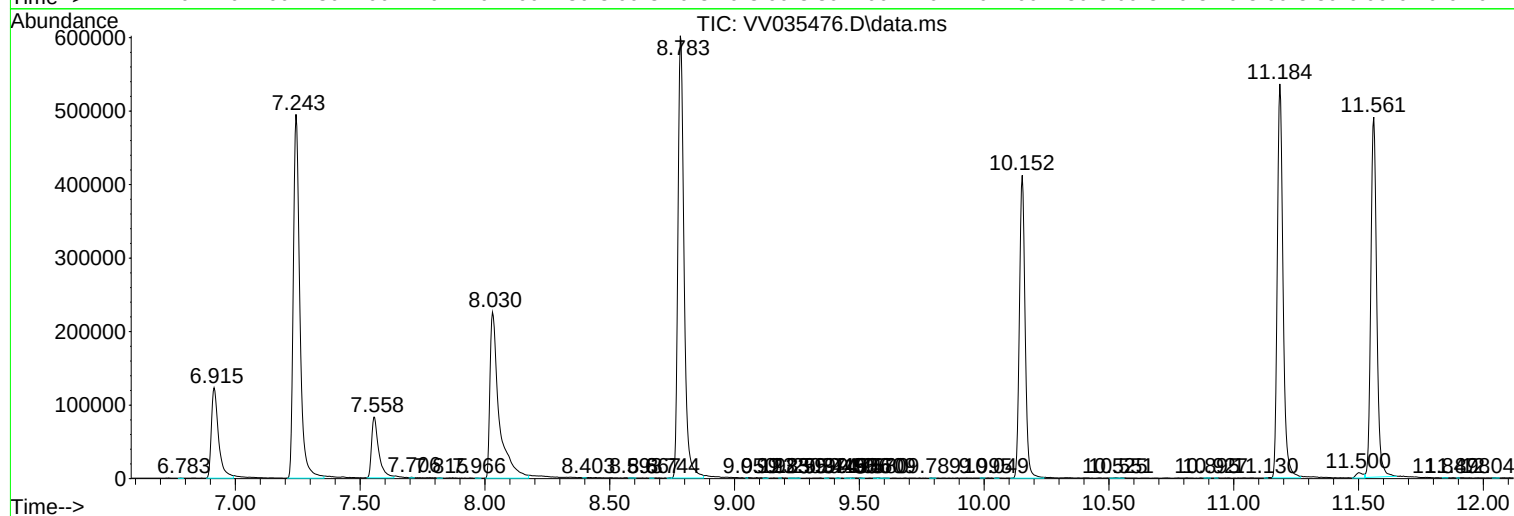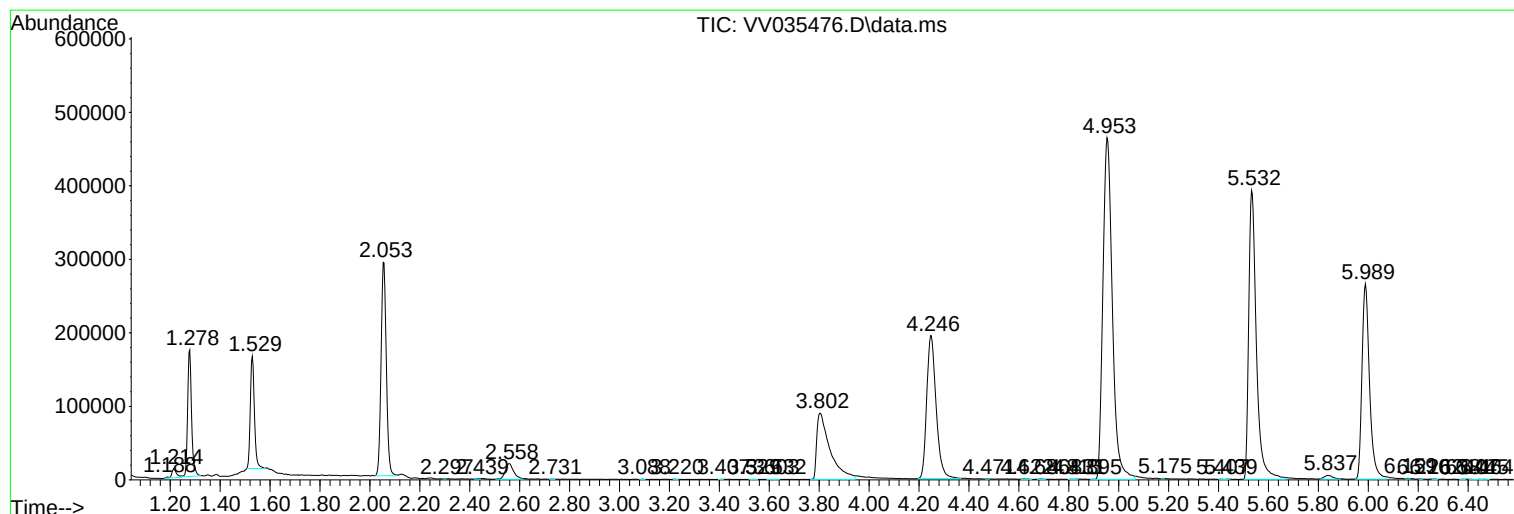

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035476.D
Acq On : 29 Apr 2024 17:21
Operator : SY/MD
Sample : P2279-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035476.D
Acq On : 29 Apr 2024 17:21
Operator : SY/MD
Sample : P2279-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc