

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035477.D
 Acq On : 29 Apr 2024 17:45
 Operator : SY/MD
 Sample : P2279-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035477.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	224343	242633	14.25%	1.842%
2	1.529	146	152	169	rVB	201708	229162	13.46%	1.740%
3	2.056	306	316	330	rBV	384275	558678	32.82%	4.242%
4	2.397	418	422	425	rBV4	659	635	0.04%	0.005%
5	2.539	462	466	467	rBV2	869	564	0.03%	0.004%
6	2.802	546	548	550	rVB	218	114	0.01%	0.001%
7	2.822	550	554	560	rBV2	278	295	0.02%	0.002%
8	2.896	569	577	580	rBV4	612	865	0.05%	0.007%
9	3.021	613	616	618	rVB2	203	118	0.01%	0.001%
10	3.037	618	621	625	rVB2	222	170	0.01%	0.001%
11	3.063	625	629	634	rBV2	241	216	0.01%	0.002%
12	3.127	645	649	652	rBV	327	215	0.01%	0.002%
13	3.204	670	673	674	rBV	225	137	0.01%	0.001%
14	3.259	687	690	691	rBV	166	81	0.00%	0.001%
15	3.314	704	707	715	rVB3	289	307	0.02%	0.002%
16	3.346	715	717	719	rBV	73	48	0.00%	0.000%
17	3.378	725	727	731	rBV2	45	38	0.00%	0.000%
18	3.407	731	736	739	rBV	256	183	0.01%	0.001%
19	3.429	742	743	745	rVB	169	59	0.00%	0.000%
20	3.452	745	750	752	rBV	267	232	0.01%	0.002%
21	3.519	769	771	773	rBV	187	85	0.00%	0.001%
22	3.542	773	778	783	rVV2	173	205	0.01%	0.002%
23	3.564	783	785	788	rVB	119	56	0.00%	0.000%
24	3.600	791	796	799	rBV2	146	155	0.01%	0.001%
25	3.664	813	816	820	rBV2	77	75	0.00%	0.001%
26	3.696	824	826	829	rBV	71	40	0.00%	0.000%
27	3.725	831	835	839	rVB2	233	203	0.01%	0.002%
28	3.748	839	842	843	rBV	153	92	0.01%	0.001%
29	3.760	843	846	847	rBV	90	37	0.00%	0.000%
30	3.799	849	858	912	rBV	112413	374994	22.03%	2.847%
31	4.246	982	997	1039	rBV2	260891	680317	39.97%	5.166%
32	4.606	1107	1109	1111	rBV2	347	123	0.01%	0.001%
33	4.638	1117	1119	1121	rBV	260	123	0.01%	0.001%
34	4.780	1159	1163	1165	rBV2	433	351	0.02%	0.003%
35	4.899	1199	1200	1201	rBV	165	52	0.00%	0.000%
36	4.953	1201	1217	1254	rBV2	629415	1702257	100.00%	12.926%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035477.D
 Acq On : 29 Apr 2024 17:45
 Operator : SY/MD
 Sample : P2279-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	5.249	1307	1309	1312	rBV4	637	323	0.02%	0.002%
38	5.397	1353	1355	1356	rBV	230	81	0.00%	0.001%
39	5.445	1368	1370	1372	rBV	245	131	0.01%	0.001%
40	5.471	1375	1378	1381	rVB2	338	180	0.01%	0.001%
41	5.532	1386	1397	1438	rBV	547080	1148670	67.48%	8.722%
42	5.985	1525	1538	1573	rBV	358435	751732	44.16%	5.708%
43	6.288	1627	1632	1638	rBV4	972	1243	0.07%	0.009%
44	6.317	1638	1641	1643	rBV2	354	232	0.01%	0.002%
45	6.333	1643	1646	1649	rVV2	373	254	0.01%	0.002%
46	6.375	1654	1659	1662	rBV3	771	598	0.04%	0.005%
47	6.394	1662	1665	1668	rBV2	272	185	0.01%	0.001%
48	6.445	1680	1681	1683	rBV	249	133	0.01%	0.001%
49	6.477	1688	1691	1693	rVB2	355	154	0.01%	0.001%
50	6.503	1696	1699	1700	rBV	162	89	0.01%	0.001%
51	6.513	1700	1702	1703	rBV	305	96	0.01%	0.001%
52	6.548	1711	1713	1715	rBV	188	75	0.00%	0.001%
53	6.571	1719	1720	1723	rVB	457	142	0.01%	0.001%
54	6.590	1723	1726	1729	rBV2	287	216	0.01%	0.002%
55	6.674	1749	1752	1755	rBV2	432	271	0.02%	0.002%
56	6.789	1785	1788	1792	rBV3	258	216	0.01%	0.002%
57	6.821	1795	1798	1800	rBV2	255	149	0.01%	0.001%
58	6.834	1800	1802	1805	rBV2	320	184	0.01%	0.001%
59	6.911	1817	1826	1852	rBV	173781	335655	19.72%	2.549%
60	7.172	1904	1907	1910	rBV3	356	233	0.01%	0.002%
61	7.243	1918	1929	1972	rBV	699546	1242748	73.01%	9.437%
62	7.555	2017	2026	2058	rBV	118027	226787	13.32%	1.722%
63	7.860	2118	2121	2123	rBV	526	319	0.02%	0.002%
64	7.918	2136	2139	2142	rVB3	632	350	0.02%	0.003%
65	7.934	2142	2144	2146	rVV	246	108	0.01%	0.001%
66	7.953	2146	2150	2152	rVB2	343	211	0.01%	0.002%
67	8.030	2164	2174	2222	rBV2	328788	789596	46.39%	5.996%
68	8.625	2357	2359	2361	rBV	281	122	0.01%	0.001%
69	8.738	2392	2394	2397	rBV2	275	119	0.01%	0.001%
70	8.783	2397	2408	2436	rBV2	859390	1618904	95.10%	12.293%
71	9.230	2541	2547	2548	rBV2	309	226	0.01%	0.002%
72	9.275	2558	2561	2562	rBV	349	202	0.01%	0.002%
73	9.397	2598	2599	2601	rBV	165	59	0.00%	0.000%
74	9.458	2614	2618	2624	rBV4	357	347	0.02%	0.003%
75	9.596	2658	2661	2662	rBV4	214	102	0.01%	0.001%
76	9.632	2669	2672	2675	rBV2	248	160	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035477.D
 Acq On : 29 Apr 2024 17:45
 Operator : SY/MD
 Sample : P2279-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	9.715	2695	2698	2699	rBV2	276	151	0.01%	0.001%
78	9.808	2725	2727	2728	rBV2	274	92	0.01%	0.001%
79	9.870	2743	2746	2749	rBV	237	174	0.01%	0.001%
80	9.956	2772	2773	2775	rVB2	143	35	0.00%	0.000%
81	10.040	2796	2799	2803	rBV	229	242	0.01%	0.002%
82	10.059	2803	2805	2806	rBV	168	74	0.00%	0.001%
83	10.153	2820	2834	2863	rBV	555812	879826	51.69%	6.681%
84	10.374	2900	2903	2905	rVB4	421	224	0.01%	0.002%
85	10.410	2911	2914	2915	rBV	422	236	0.01%	0.002%
86	10.509	2942	2945	2949	rVB2	549	411	0.02%	0.003%
87	10.532	2949	2952	2954	rBV	197	115	0.01%	0.001%
88	10.564	2959	2962	2966	rBV	330	219	0.01%	0.002%
89	10.757	3020	3022	3025	rVB	311	159	0.01%	0.001%
90	11.130	3130	3138	3144	rBV3	5743	8898	0.52%	0.068%
91	11.185	3144	3155	3187	rVB	748251	1234391	72.51%	9.373%
92	11.558	3260	3271	3299	rBV	686495	1126241	66.16%	8.552%
93	11.837	3354	3358	3360	rBV2	525	470	0.03%	0.004%
94	11.895	3374	3376	3378	rBV	344	180	0.01%	0.001%
95	11.943	3390	3391	3392	rBV	290	80	0.00%	0.001%
96	11.998	3406	3408	3411	rBV	359	277	0.02%	0.002%
97	12.294	3497	3500	3503	rBV2	358	238	0.01%	0.002%
98	12.371	3522	3524	3526	rBV	312	179	0.01%	0.001%
99	12.397	3529	3532	3537	rBV3	650	518	0.03%	0.004%
100	13.172	3770	3773	3775	rBV	479	293	0.02%	0.002%




Sum of corrected areas: 13169240

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035477.D
Acq On : 29 Apr 2024 17:45
Operator : SY/MD
Sample : P2279-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

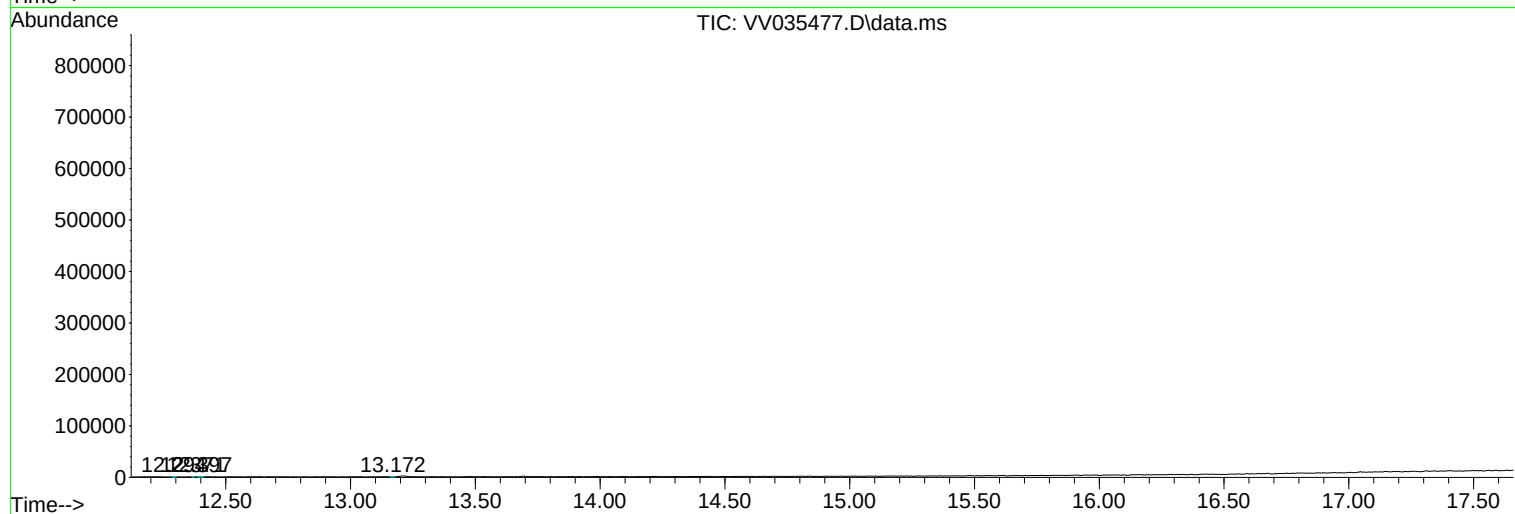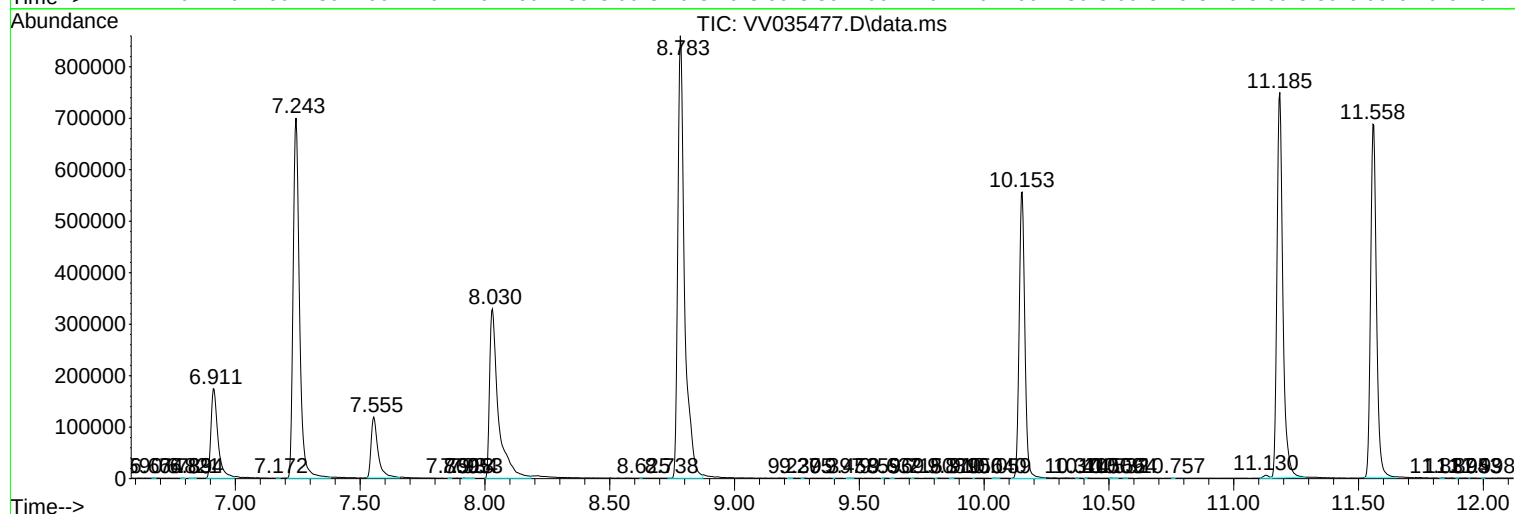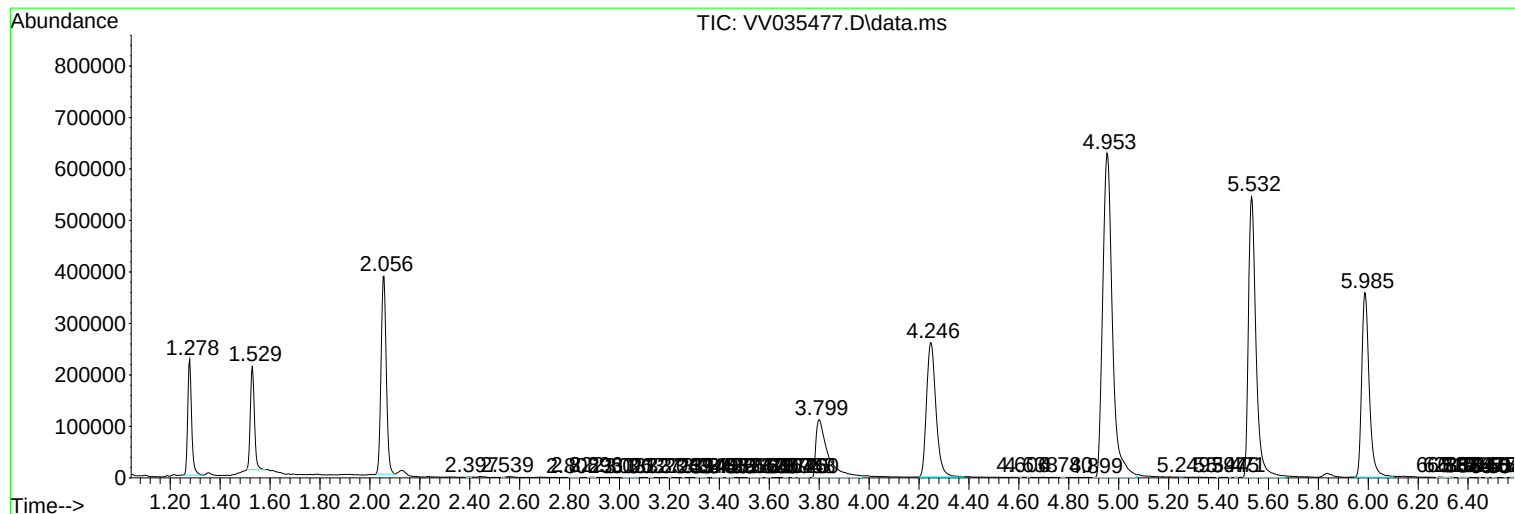

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035477.D
Acq On : 29 Apr 2024 17:45
Operator : SY/MD
Sample : P2279-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035477.D
Acq On : 29 Apr 2024 17:45
Operator : SY/MD
Sample : P2279-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
