

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035478.D
 Acq On : 29 Apr 2024 18:09
 Operator : SY/MD
 Sample : P2279-13DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	40	46	49	rBV	2338	2538	0.11%	0.017%
2	1.214	49	54	61	rVV2	3688	5180	0.23%	0.034%
3	1.278	66	74	90	rVV	218062	245243	11.09%	1.598%
4	1.529	145	152	166	rBV	206685	238391	10.78%	1.554%
5	2.053	305	315	333	rBV	380197	552673	24.99%	3.602%
6	2.301	389	392	393	rBV2	424	212	0.01%	0.001%
7	2.330	397	401	404	rBV3	715	661	0.03%	0.004%
8	2.384	416	418	423	rVB3	351	228	0.01%	0.001%
9	2.449	430	438	447	rVB2	4438	6882	0.31%	0.045%
10	2.558	461	472	488	rBV2	4802	11032	0.50%	0.072%
11	2.674	504	508	511	rVB2	451	331	0.01%	0.002%
12	2.709	516	519	523	rVV2	404	374	0.02%	0.002%
13	2.744	526	530	535	rBV2	297	267	0.01%	0.002%
14	2.770	535	538	540	rBV	379	244	0.01%	0.002%
15	2.812	548	551	555	rVB3	389	265	0.01%	0.002%
16	2.886	569	574	575	rBV3	404	270	0.01%	0.002%
17	2.905	578	580	584	rVB2	322	200	0.01%	0.001%
18	3.101	634	641	644	rBV2	242	233	0.01%	0.002%
19	3.291	697	700	709	rVB2	280	386	0.02%	0.003%
20	3.359	717	721	724	rBV2	310	213	0.01%	0.001%
21	3.735	833	838	843	rVB2	244	230	0.01%	0.001%
22	3.802	850	859	907	rBV2	116553	397120	17.95%	2.588%
23	4.146	963	966	967	rBV2	558	322	0.01%	0.002%
24	4.246	980	997	1027	rBV	263281	685346	30.98%	4.466%
25	4.519	1080	1082	1088	rVB4	346	315	0.01%	0.002%
26	4.548	1089	1091	1095	rVB3	445	253	0.01%	0.002%
27	4.953	1201	1217	1269	rBV2	641537	1681343	76.01%	10.957%
28	5.217	1295	1299	1300	rBV3	544	320	0.01%	0.002%
29	5.262	1311	1313	1317	rBV2	358	225	0.01%	0.001%
30	5.326	1332	1333	1338	rVB2	329	233	0.01%	0.002%
31	5.391	1350	1353	1358	rVB2	488	373	0.02%	0.002%
32	5.420	1358	1362	1364	rBV2	208	191	0.01%	0.001%
33	5.532	1386	1397	1440	rBV	541078	1131856	51.17%	7.376%
34	5.834	1481	1491	1503	rBV4	6566	14534	0.66%	0.095%
35	5.921	1516	1518	1521	rBV2	340	234	0.01%	0.002%
36	5.986	1526	1538	1568	rBV	366430	764084	34.54%	4.979%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035478.D
 Acq On : 29 Apr 2024 18:09
 Operator : SY/MD
 Sample : P2279-13DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.294	1631	1634	1636	rVV3	516	235	0.01%	0.002%
38	6.307	1636	1638	1644	rVB3	354	304	0.01%	0.002%
39	6.336	1644	1647	1650	rBV	353	249	0.01%	0.002%
40	6.407	1664	1669	1672	rBV	432	282	0.01%	0.002%
41	6.551	1710	1714	1717	rBV	277	192	0.01%	0.001%
42	6.667	1744	1750	1752	rBV	304	217	0.01%	0.001%
43	6.825	1795	1799	1805	rVB2	201	240	0.01%	0.002%
44	6.912	1816	1826	1862	rBV	173616	345307	15.61%	2.250%
45	7.191	1909	1913	1916	rVB4	322	233	0.01%	0.002%
46	7.243	1918	1929	1959	rBV	695805	1229809	55.60%	8.014%
47	7.555	2016	2026	2059	rBV	122630	236243	10.68%	1.540%
48	7.863	2119	2122	2124	rBV3	399	243	0.01%	0.002%
49	7.928	2136	2142	2145	rBV3	444	353	0.02%	0.002%
50	7.953	2148	2150	2153	rBV3	275	206	0.01%	0.001%
51	7.998	2161	2164	2165	rBV2	336	197	0.01%	0.001%
52	8.030	2165	2174	2218	rBV2	351059	826698	37.38%	5.387%
53	8.407	2288	2291	2294	rVB3	414	301	0.01%	0.002%
54	8.432	2295	2299	2301	rVB4	536	339	0.02%	0.002%
55	8.490	2315	2317	2320	rBV2	369	262	0.01%	0.002%
56	8.526	2326	2328	2331	rVB2	486	219	0.01%	0.001%
57	8.548	2331	2335	2336	rBV3	606	429	0.02%	0.003%
58	8.664	2369	2371	2373	rVV2	453	247	0.01%	0.002%
59	8.715	2382	2387	2391	rBV4	451	419	0.02%	0.003%
60	8.783	2396	2408	2442	rBV	842053	1483361	67.06%	9.667%
61	9.030	2482	2485	2489	rBV4	568	459	0.02%	0.003%
62	9.072	2493	2498	2502	rVB4	440	412	0.02%	0.003%
63	9.104	2506	2508	2510	rBV2	468	238	0.01%	0.002%
64	9.201	2532	2538	2542	rVB2	427	431	0.02%	0.003%
65	9.255	2552	2555	2556	rBV2	497	203	0.01%	0.001%
66	9.323	2574	2576	2579	rBV2	691	341	0.02%	0.002%
67	9.574	2650	2654	2659	rBV3	392	337	0.02%	0.002%
68	9.683	2685	2688	2697	rVB3	331	363	0.02%	0.002%
69	9.886	2748	2751	2756	rVB2	336	243	0.01%	0.002%
70	9.915	2756	2760	2763	rVB2	290	192	0.01%	0.001%
71	9.944	2767	2769	2773	rVV2	320	221	0.01%	0.001%
72	10.082	2808	2812	2815	rBV3	283	205	0.01%	0.001%
73	10.149	2821	2833	2868	rBV	575233	915008	41.37%	5.963%
74	10.326	2885	2888	2892	rVB4	389	277	0.01%	0.002%
75	10.480	2931	2936	2939	rVB3	391	227	0.01%	0.001%
76	10.715	3007	3009	3013	rVB2	356	199	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035478.D
 Acq On : 29 Apr 2024 18:09
 Operator : SY/MD
 Sample : P2279-13DL 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR6DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	10.789	3031	3032	3037	rVB2	735	505	0.02%	0.003%
78	10.818	3037	3041	3043	rBV2	314	239	0.01%	0.002%
79	11.120	3125	3135	3145	rBV	96024	156035	7.05%	1.017%
80	11.185	3145	3155	3187	rVB2	811875	1649623	74.58%	10.750%
81	11.452	3236	3238	3242	rVB	307	232	0.01%	0.002%
82	11.564	3259	3273	3301	rBV2	948100	2211868	100.00%	14.414%
83	11.979	3399	3402	3406	rVB3	500	337	0.02%	0.002%
84	12.053	3422	3425	3428	rBV2	415	340	0.02%	0.002%
85	12.082	3431	3434	3438	rVB2	487	364	0.02%	0.002%
86	12.191	3464	3468	3471	rBV3	336	234	0.01%	0.002%
87	12.255	3485	3488	3496	rVB3	427	465	0.02%	0.003%
88	12.603	3593	3596	3601	rVB3	613	413	0.02%	0.003%
89	12.641	3605	3608	3612	rBV4	462	348	0.02%	0.002%
90	12.805	3653	3659	3660	rBV2	342	270	0.01%	0.002%
91	12.844	3669	3671	3673	rBV3	520	309	0.01%	0.002%
92	12.914	3688	3693	3695	rBV	320	348	0.02%	0.002%
93	12.947	3700	3703	3708	rVB2	535	489	0.02%	0.003%
94	12.988	3714	3716	3720	rBV2	427	319	0.01%	0.002%
95	13.050	3732	3735	3738	rBV2	422	258	0.01%	0.002%
96	13.140	3760	3763	3768	rVB	410	289	0.01%	0.002%
97	13.197	3770	3781	3803	rBV	210478	335967	15.19%	2.189%
98	13.680	3920	3931	3950	rBV	119655	195774	8.85%	1.276%
99	13.934	4006	4010	4012	rBV4	461	418	0.02%	0.003%
100	14.111	4062	4065	4068	rBV4	852	618	0.03%	0.004%




Sum of corrected areas: 15344805

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035478.D
Acq On : 29 Apr 2024 18:09
Operator : SY/MD
Sample : P2279-13DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

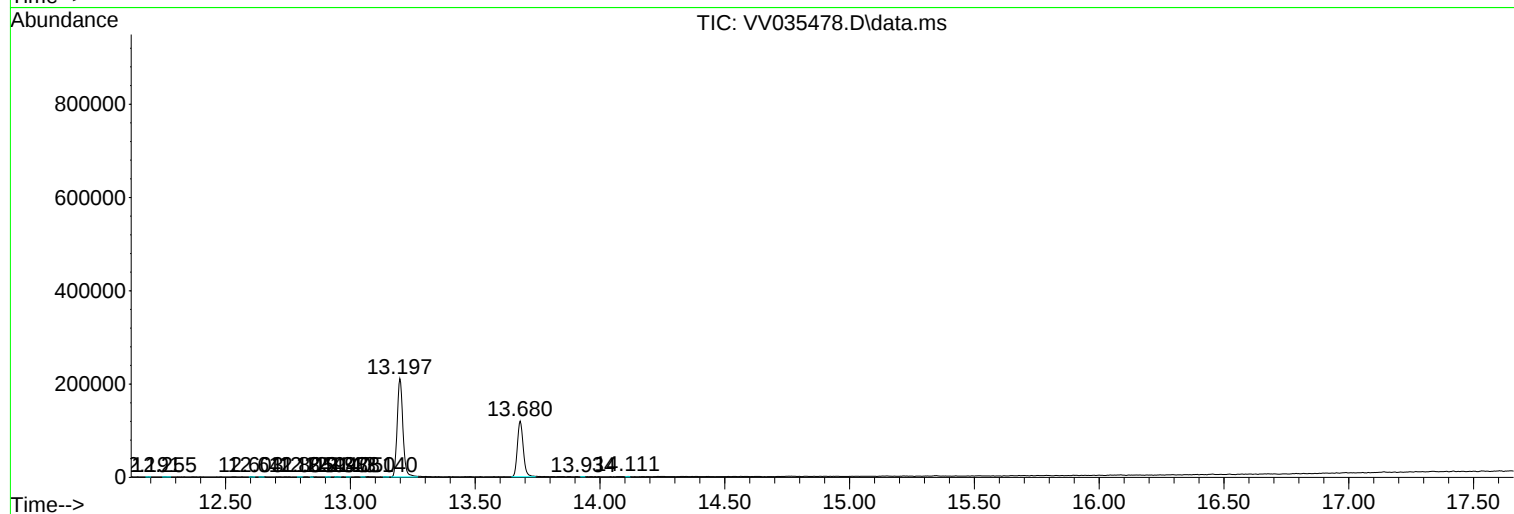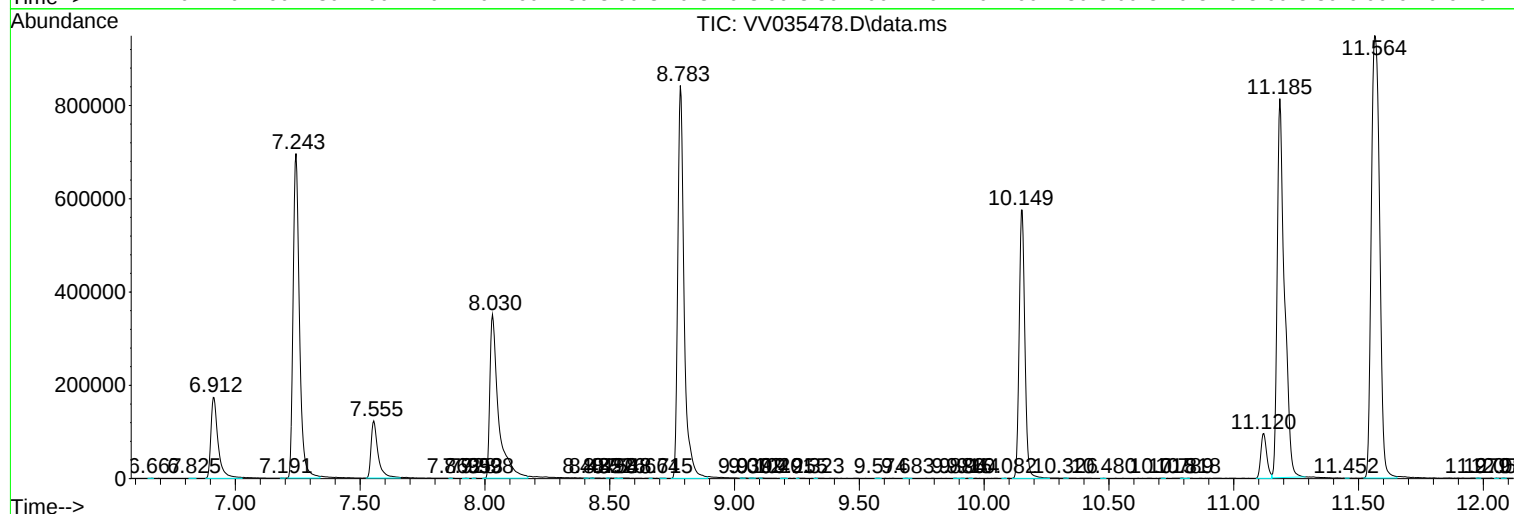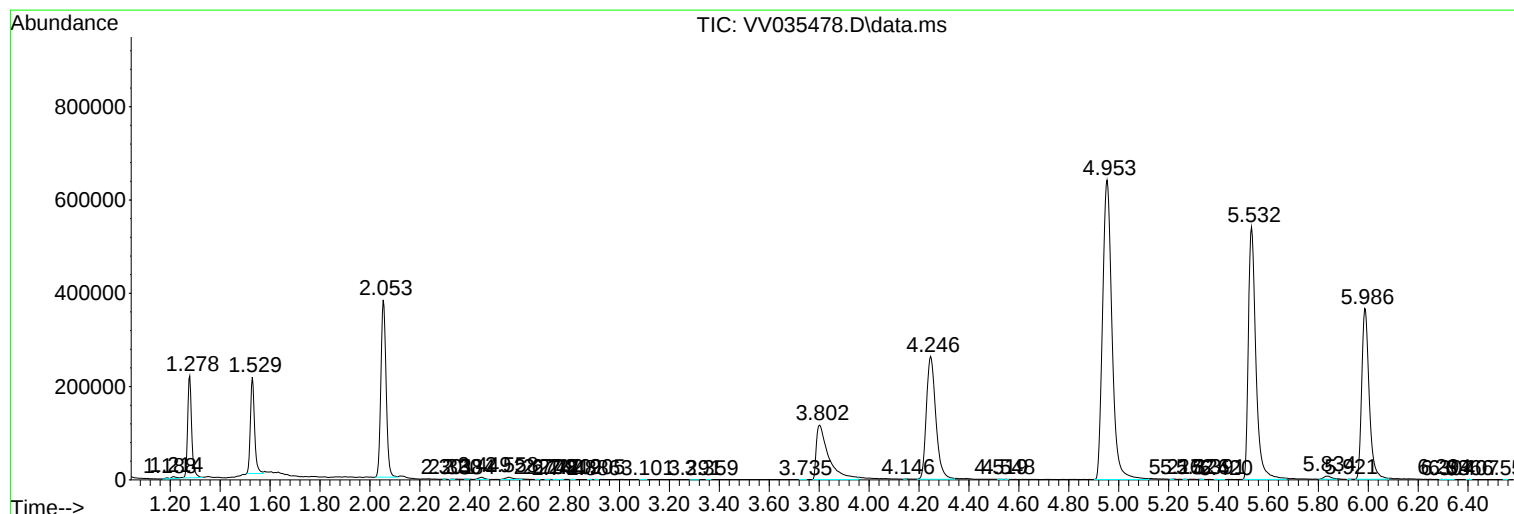

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035478.D
Acq On : 29 Apr 2024 18:09
Operator : SY/MD
Sample : P2279-13DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035478.D
Acq On : 29 Apr 2024 18:09
Operator : SY/MD
Sample : P2279-13DL 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
