

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035480.D
 Acq On : 29 Apr 2024 18:57
 Operator : SY/MD
 Sample : P2279-12 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035480.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	66	74	92	rVB	225367	244361	7.39%	1.519%
2	1.529	145	152	170	rBV	207561	240192	7.27%	1.494%
3	2.053	305	315	333	rBV	381879	556574	16.84%	3.461%
4	2.278	382	385	390	rBV2	414	340	0.01%	0.002%
5	2.304	390	393	396	rVV2	462	375	0.01%	0.002%
6	2.330	399	401	404	rVB2	537	266	0.01%	0.002%
7	2.362	409	411	417	rBV3	558	503	0.02%	0.003%
8	2.449	430	438	446	rVB3	3372	5272	0.16%	0.033%
9	2.555	463	471	493	rVB	4990	11157	0.34%	0.069%
10	2.683	509	511	514	rBV3	354	246	0.01%	0.002%
11	2.719	519	522	524	rVB2	438	278	0.01%	0.002%
12	2.751	530	532	537	rVB2	322	228	0.01%	0.001%
13	2.937	587	590	593	rVV2	323	237	0.01%	0.001%
14	3.047	622	624	629	rVB2	350	237	0.01%	0.001%
15	3.079	629	634	638	rBV3	270	254	0.01%	0.002%
16	3.272	690	694	699	rBV3	404	387	0.01%	0.002%
17	3.375	721	726	730	rBV2	352	293	0.01%	0.002%
18	3.555	778	782	787	rVB	509	351	0.01%	0.002%
19	3.741	836	840	845	rVB2	322	245	0.01%	0.002%
20	3.802	850	859	909	rBV	118115	405778	12.28%	2.523%
21	4.246	981	997	1025	rBV	272701	723307	21.88%	4.498%
22	4.484	1069	1071	1077	rVB3	553	396	0.01%	0.002%
23	4.519	1077	1082	1084	rBV3	408	322	0.01%	0.002%
24	4.580	1099	1101	1105	rVB2	400	304	0.01%	0.002%
25	4.728	1144	1147	1149	rBV3	378	224	0.01%	0.001%
26	4.744	1149	1152	1157	rVB4	371	314	0.01%	0.002%
27	4.802	1167	1170	1174	rVB2	352	270	0.01%	0.002%
28	4.825	1174	1177	1182	rBV2	345	284	0.01%	0.002%
29	4.854	1182	1186	1189	rBV3	313	217	0.01%	0.001%
30	4.953	1201	1217	1227	rBV2	655898	1661853	50.28%	10.334%
31	5.388	1348	1352	1356	rBV2	295	258	0.01%	0.002%
32	5.439	1361	1368	1370	rBV4	603	639	0.02%	0.004%
33	5.532	1386	1397	1445	rBV	568556	1199714	36.30%	7.460%
34	5.834	1481	1491	1506	rVV7	6447	14613	0.44%	0.091%
35	5.934	1519	1522	1524	rVV3	558	344	0.01%	0.002%
36	5.986	1525	1538	1567	rVV	364939	767515	23.22%	4.773%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035480.D
 Acq On : 29 Apr 2024 18:57
 Operator : SY/MD
 Sample : P2279-12 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.162	1590	1593	1597	rVB5	1016	789	0.02%	0.005%
38	6.288	1630	1632	1637	rVB3	546	305	0.01%	0.002%
39	6.359	1652	1654	1656	rBV	501	306	0.01%	0.002%
40	6.371	1656	1658	1661	rVV2	542	295	0.01%	0.002%
41	6.391	1661	1664	1670	rVB	456	288	0.01%	0.002%
42	6.674	1749	1752	1754	rVV	380	213	0.01%	0.001%
43	6.709	1757	1763	1765	rVV3	413	398	0.01%	0.002%
44	6.751	1770	1776	1779	rVB2	479	365	0.01%	0.002%
45	6.912	1814	1826	1868	rBV	176162	354611	10.73%	2.205%
46	7.079	1877	1878	1884	rVB4	606	419	0.01%	0.003%
47	7.243	1918	1929	1967	rVV	713325	1278082	38.67%	7.947%
48	7.432	1985	1988	1994	rVB3	1154	1077	0.03%	0.007%
49	7.555	2013	2026	2054	rBV	124441	238981	7.23%	1.486%
50	7.751	2085	2087	2091	rVB3	759	369	0.01%	0.002%
51	7.812	2103	2106	2110	rVB3	278	222	0.01%	0.001%
52	7.867	2121	2123	2128	rVB3	327	248	0.01%	0.002%
53	7.921	2136	2140	2143	rBV3	420	352	0.01%	0.002%
54	7.979	2156	2158	2163	rVB3	285	214	0.01%	0.001%
55	8.030	2165	2174	2228	rBV2	353605	845417	25.58%	5.257%
56	8.561	2335	2339	2341	rBV3	470	352	0.01%	0.002%
57	8.657	2365	2369	2376	rVB4	362	457	0.01%	0.003%
58	8.693	2376	2380	2381	rBV2	633	398	0.01%	0.002%
59	8.783	2395	2408	2413	rBV	936119	1518314	45.94%	9.441%
60	9.101	2503	2507	2508	rBV3	469	319	0.01%	0.002%
61	9.137	2516	2518	2523	rBV3	402	294	0.01%	0.002%
62	9.204	2535	2539	2542	rVB2	408	304	0.01%	0.002%
63	9.227	2542	2546	2549	rBV3	384	343	0.01%	0.002%
64	9.265	2553	2558	2564	rVB5	512	498	0.02%	0.003%
65	9.326	2573	2577	2583	rVV2	443	448	0.01%	0.003%
66	9.419	2604	2606	2612	rVB2	317	312	0.01%	0.002%
67	9.458	2612	2618	2621	rBV2	357	238	0.01%	0.001%
68	9.513	2632	2635	2640	rBV3	413	340	0.01%	0.002%
69	9.969	2773	2777	2779	rBV	358	258	0.01%	0.002%
70	10.108	2815	2820	2821	rBV2	287	219	0.01%	0.001%
71	10.153	2822	2834	2859	rBV	576668	924663	27.98%	5.750%
72	10.275	2869	2872	2878	rVB4	419	319	0.01%	0.002%
73	10.448	2922	2926	2929	rVB2	421	294	0.01%	0.002%
74	10.789	3030	3032	3039	rVB4	638	546	0.02%	0.003%
75	10.985	3088	3093	3098	rVV3	275	356	0.01%	0.002%
76	11.069	3113	3119	3124	rBV3	318	392	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035480.D
 Acq On : 29 Apr 2024 18:57
 Operator : SY/MD
 Sample : P2279-12 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	11.117	3124	3134	3145	rBV	146796	231168	6.99%	1.437%
78	11.185	3145	3155	3159	rBV	914777	1392986	42.15%	8.662%
79	11.477	3243	3246	3249	rVB4	841	602	0.02%	0.004%
80	11.574	3259	3276	3307	rBV2	1524837	3305057	100.00%	20.552%
81	11.873	3367	3369	3375	rVB5	440	291	0.01%	0.002%
82	12.188	3463	3467	3472	rVB2	530	425	0.01%	0.003%
83	12.564	3582	3584	3587	rBV2	432	253	0.01%	0.002%
84	12.603	3590	3596	3598	rBV4	1436	1550	0.05%	0.010%
85	12.744	3638	3640	3644	rVB2	497	358	0.01%	0.002%
86	12.773	3644	3649	3655	rBV3	540	547	0.02%	0.003%
87	12.808	3656	3660	3663	rVB3	381	279	0.01%	0.002%
88	12.985	3711	3715	3719	rVB2	572	478	0.01%	0.003%
89	13.053	3733	3736	3739	rVB2	536	316	0.01%	0.002%
90	13.201	3772	3782	3800	rBV2	55575	90651	2.74%	0.564%
91	13.291	3808	3810	3812	rBV2	440	217	0.01%	0.001%
92	13.683	3923	3932	3944	rBV2	27140	42727	1.29%	0.266%
93	13.754	3951	3954	3957	rBV3	430	296	0.01%	0.002%
94	13.886	3992	3995	3998	rBV3	586	533	0.02%	0.003%
95	13.927	4006	4008	4012	rBV3	378	271	0.01%	0.002%
96	13.966	4018	4020	4023	rBV2	309	215	0.01%	0.001%
97	14.033	4039	4041	4045	rBV2	338	221	0.01%	0.001%
98	14.377	4146	4148	4154	rVB3	583	469	0.01%	0.003%
99	14.429	4161	4164	4168	rVB2	591	505	0.02%	0.003%
100	14.468	4172	4176	4178	rBV2	693	545	0.02%	0.003%




Sum of corrected areas: 16081723

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035480.D
Acq On : 29 Apr 2024 18:57
Operator : SY/MD
Sample : P2279-12 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

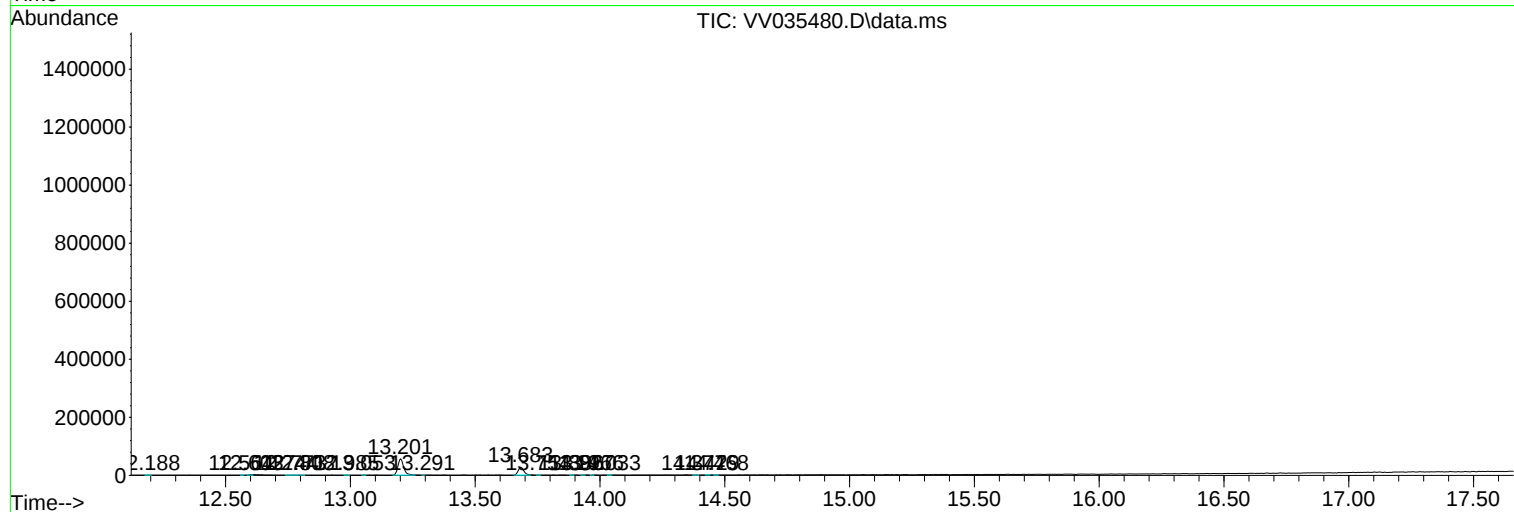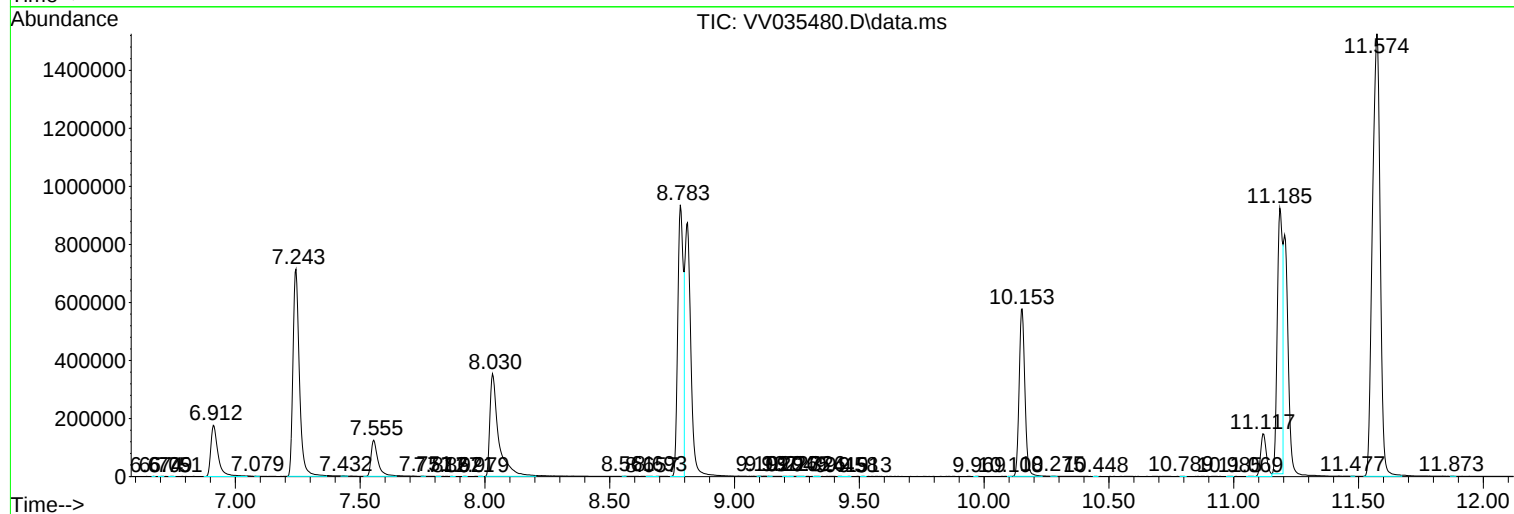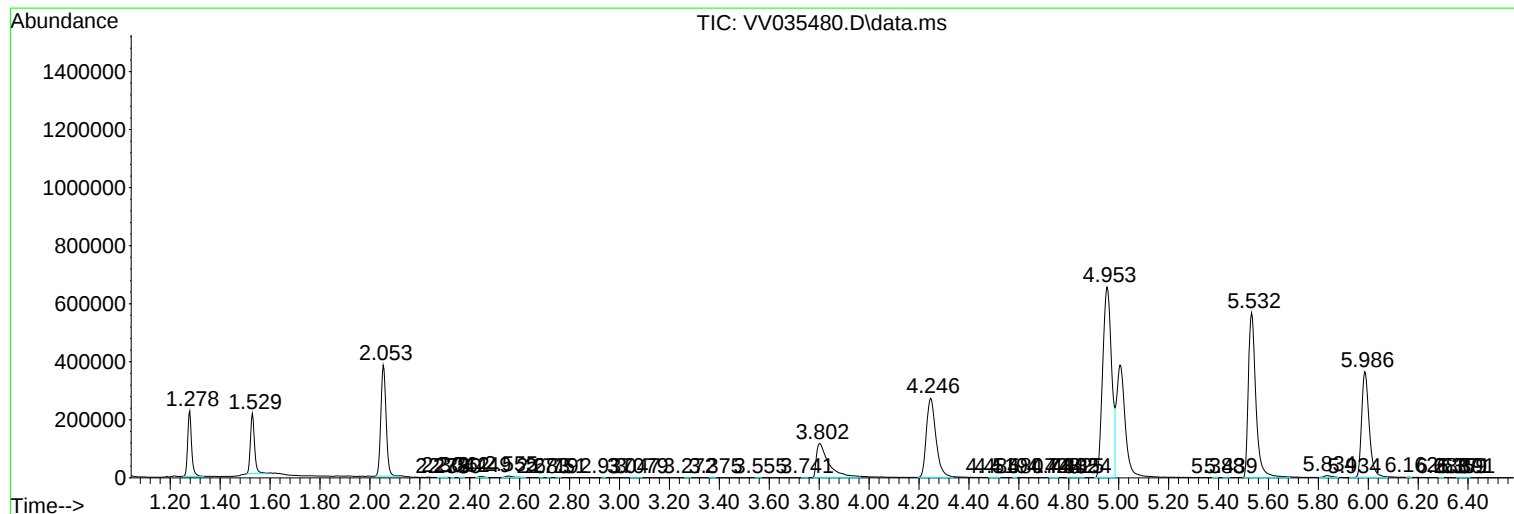

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035480.D
Acq On : 29 Apr 2024 18:57
Operator : SY/MD
Sample : P2279-12 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035480.D
Acq On : 29 Apr 2024 18:57
Operator : SY/MD
Sample : P2279-12 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------