

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035481.D
 Acq On : 29 Apr 2024 19:21
 Operator : SY/MD
 Sample : P2279-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035481.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	49	54	64	rBV	14210	16569	0.08%	0.025%
2	1.278	67	74	93	rVB	221754	245483	1.14%	0.377%
3	1.529	146	152	164	rBV	194509	225049	1.04%	0.345%
4	2.053	306	315	334	rVB	389329	557084	2.58%	0.854%
5	2.555	463	471	473	rBV4	866	1184	0.01%	0.002%
6	2.690	511	513	516	rBV2	347	201	0.00%	0.000%
7	2.883	567	573	577	rBV2	343	372	0.00%	0.001%
8	2.902	577	579	581	rBV	165	82	0.00%	0.000%
9	3.024	614	617	620	rBV2	139	97	0.00%	0.000%
10	3.085	633	636	640	rBV3	237	201	0.00%	0.000%
11	3.150	651	656	660	rVV3	217	197	0.00%	0.000%
12	3.169	660	662	666	rVV2	246	189	0.00%	0.000%
13	3.201	668	672	675	rVB2	317	221	0.00%	0.000%
14	3.227	677	680	682	rBV	228	151	0.00%	0.000%
15	3.281	694	697	702	rVB2	298	248	0.00%	0.000%
16	3.359	717	721	729	rVB2	321	267	0.00%	0.000%
17	3.445	745	748	752	rBV2	207	164	0.00%	0.000%
18	3.461	752	753	757	rVB	155	77	0.00%	0.000%
19	3.516	767	770	772	rBV	131	107	0.00%	0.000%
20	3.574	783	788	789	rBV2	201	147	0.00%	0.000%
21	3.609	796	799	802	rBV	147	108	0.00%	0.000%
22	3.648	807	811	813	rBV2	332	210	0.00%	0.000%
23	3.674	816	819	820	rBV2	354	172	0.00%	0.000%
24	3.709	828	830	832	rVB2	266	107	0.00%	0.000%
25	3.731	832	837	840	rBV	303	218	0.00%	0.000%
26	3.802	850	859	902	rBV	106842	358461	1.66%	0.550%
27	4.246	982	997	1030	rBV	260285	675824	3.13%	1.037%
28	4.590	1101	1104	1107	rBV3	552	315	0.00%	0.000%
29	4.654	1120	1124	1128	rBV3	393	440	0.00%	0.001%
30	4.690	1134	1135	1137	rVB	255	72	0.00%	0.000%
31	4.706	1137	1140	1141	rBV	455	274	0.00%	0.000%
32	4.841	1179	1182	1185	rBV2	299	255	0.00%	0.000%
33	4.953	1201	1217	1262	rBV2	629483	1663961	7.72%	2.552%
34	5.394	1351	1354	1355	rBV2	246	139	0.00%	0.000%
35	5.468	1375	1377	1379	rVB	379	148	0.00%	0.000%
36	5.532	1386	1397	1428	rBV	546879	1132709	5.25%	1.737%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035481.D
 Acq On : 29 Apr 2024 19:21
 Operator : SY/MD
 Sample : P2279-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	5.924	1517	1519	1524	rBV2	494	434	0.00%	0.001%
38	5.985	1526	1538	1571	rVV	351816	746546	3.46%	1.145%
39	6.336	1643	1647	1650	rBV3	548	421	0.00%	0.001%
40	6.374	1654	1659	1661	rBV3	392	345	0.00%	0.001%
41	6.400	1666	1667	1669	rBV	168	71	0.00%	0.000%
42	6.461	1683	1686	1691	rBV3	443	396	0.00%	0.001%
43	6.493	1694	1696	1699	rVB	280	132	0.00%	0.000%
44	6.513	1699	1702	1706	rVB2	125	98	0.00%	0.000%
45	6.535	1706	1709	1711	rBV	287	148	0.00%	0.000%
46	6.600	1726	1729	1732	rVB2	266	142	0.00%	0.000%
47	6.661	1745	1748	1749	rBV2	363	177	0.00%	0.000%
48	6.686	1752	1756	1761	rVV2	262	237	0.00%	0.000%
49	6.725	1766	1768	1771	rVB2	270	119	0.00%	0.000%
50	6.747	1771	1775	1777	rBV2	419	204	0.00%	0.000%
51	6.757	1777	1778	1781	rBV	125	68	0.00%	0.000%
52	6.911	1816	1826	1863	rBV	167716	339881	1.58%	0.521%
53	7.133	1892	1895	1898	rBV3	474	351	0.00%	0.001%
54	7.243	1918	1929	1968	rBV	700982	1257837	5.83%	1.929%
55	7.554	2017	2026	2055	rBV	120594	229071	1.06%	0.351%
56	7.828	2108	2111	2112	rBV	714	253	0.00%	0.000%
57	7.963	2149	2153	2154	rBV	374	298	0.00%	0.000%
58	7.992	2158	2162	2164	rBV3	219	204	0.00%	0.000%
59	8.030	2164	2174	2226	rBV2	337390	800930	3.71%	1.229%
60	8.435	2296	2300	2302	rBV4	550	352	0.00%	0.001%
61	8.558	2336	2338	2341	rVB3	582	307	0.00%	0.000%
62	8.680	2374	2376	2377	rBV	236	103	0.00%	0.000%
63	8.783	2396	2408	2412	rBV	936096	1397928	6.48%	2.144%
64	9.104	2506	2508	2509	rBV2	453	180	0.00%	0.000%
65	9.185	2531	2533	2534	rBV	345	114	0.00%	0.000%
66	9.210	2537	2541	2545	rVV5	459	457	0.00%	0.001%
67	9.233	2545	2548	2551	rVV2	417	246	0.00%	0.000%
68	9.249	2551	2553	2557	rVB2	587	333	0.00%	0.001%
69	9.268	2557	2559	2565	rBV4	444	404	0.00%	0.001%
70	9.397	2597	2599	2600	rBV	210	78	0.00%	0.000%
71	9.513	2632	2635	2636	rBV	162	85	0.00%	0.000%
72	9.599	2658	2662	2665	rBV2	515	401	0.00%	0.001%
73	9.709	2694	2696	2698	rVB2	320	129	0.00%	0.000%
74	9.728	2698	2702	2704	rBV	308	288	0.00%	0.000%
75	9.808	2723	2727	2730	rVB3	466	301	0.00%	0.000%
76	9.834	2732	2735	2737	rBV3	192	125	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
 Data File : VV035481.D
 Acq On : 29 Apr 2024 19:21
 Operator : SY/MD
 Sample : P2279-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	9.960	2770	2774	2775	rBV2	175	132	0.00%	0.000%
78	10.001	2781	2787	2790	rBV3	411	448	0.00%	0.001%
79	10.053	2799	2803	2805	rBV2	388	277	0.00%	0.000%
80	10.152	2822	2834	2858	rBV	566762	906373	4.20%	1.390%
81	10.419	2915	2917	2919	rBV3	228	118	0.00%	0.000%
82	10.429	2919	2920	2921	rBV3	353	113	0.00%	0.000%
83	10.554	2952	2959	2961	rBV3	266	302	0.00%	0.000%
84	10.599	2970	2973	2976	rBV	287	164	0.00%	0.000%
85	10.619	2976	2979	2981	rBV3	305	180	0.00%	0.000%
86	10.751	3018	3020	3022	rBV	252	123	0.00%	0.000%
87	10.792	3030	3033	3035	rBV2	485	323	0.00%	0.000%
88	10.821	3040	3042	3047	rVB3	305	213	0.00%	0.000%
89	10.937	3075	3078	3079	rBV	213	129	0.00%	0.000%
90	10.953	3079	3083	3087	rVV3	442	378	0.00%	0.001%
91	11.114	3121	3133	3146	rBV	2545790	3819614	17.72%	5.859%
92	11.207	3146	3162	3192	rVB2	6995257	11978418	55.56%	18.373%
93	11.577	3261	3277	3302	rBV2	13449350	21560178	100.00%	33.071%
94	12.249	3484	3486	3487	rBV2	508	161	0.00%	0.000%
95	12.435	3542	3544	3547	rVB3	528	263	0.00%	0.000%
96	13.088	3744	3747	3749	rBV2	626	459	0.00%	0.001%
97	13.194	3767	3780	3815	rBV	7797581	11491419	53.30%	17.626%
98	13.676	3917	3930	3964	rBV	3632469	5575917	25.86%	8.553%
99	14.757	4253	4266	4280	rVB2	48179	98117	0.46%	0.150%
100	15.332	4437	4445	4461	rVB	61372	98692	0.46%	0.151%




Sum of corrected areas: 65194208

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035481.D
Acq On : 29 Apr 2024 19:21
Operator : SY/MD
Sample : P2279-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

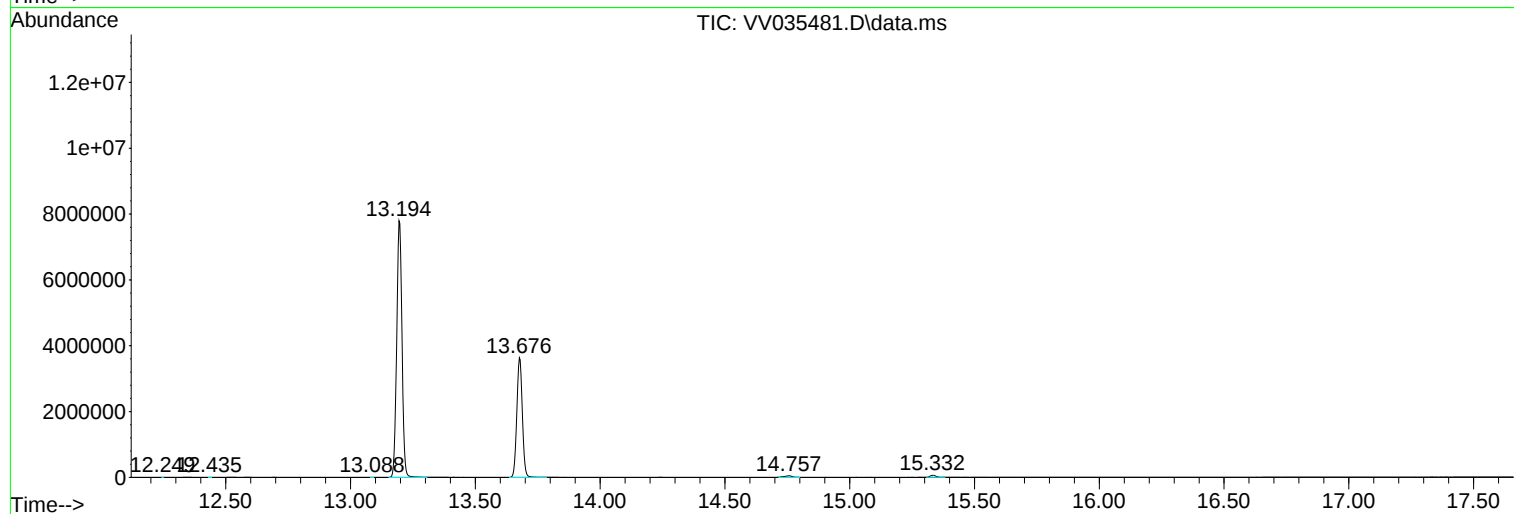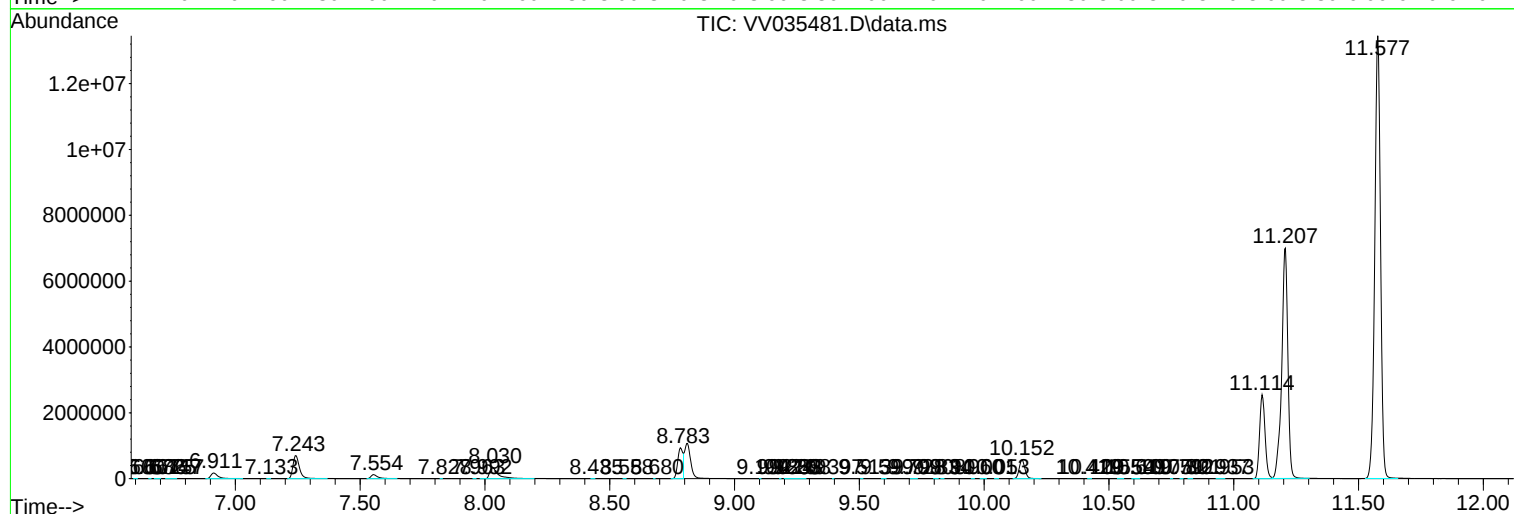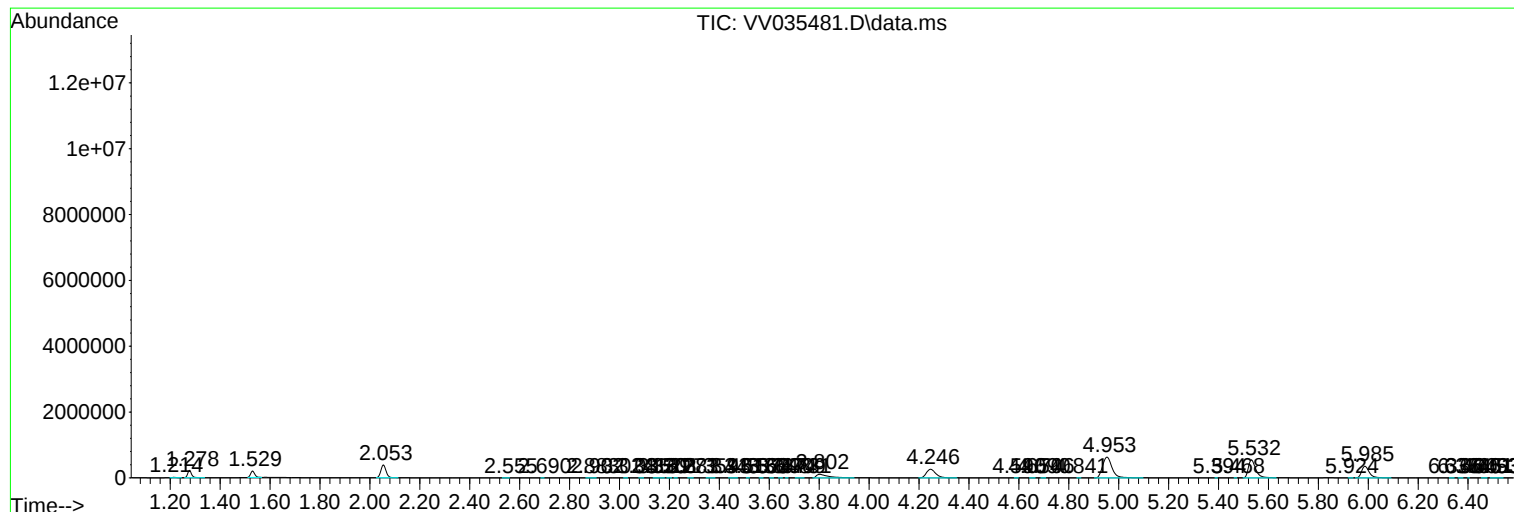

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035481.D
Acq On : 29 Apr 2024 19:21
Operator : SY/MD
Sample : P2279-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035481.D
Acq On : 29 Apr 2024 19:21
Operator : SY/MD
Sample : P2279-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
