


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042924\
Data File : VV035457.D
Acq On : 29 Apr 2024 08:52
Operator : SY/MD
Sample : BFB293
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB293

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Title : VOC Analysis
Last Update : Tue Apr 30 02:09:05 2024

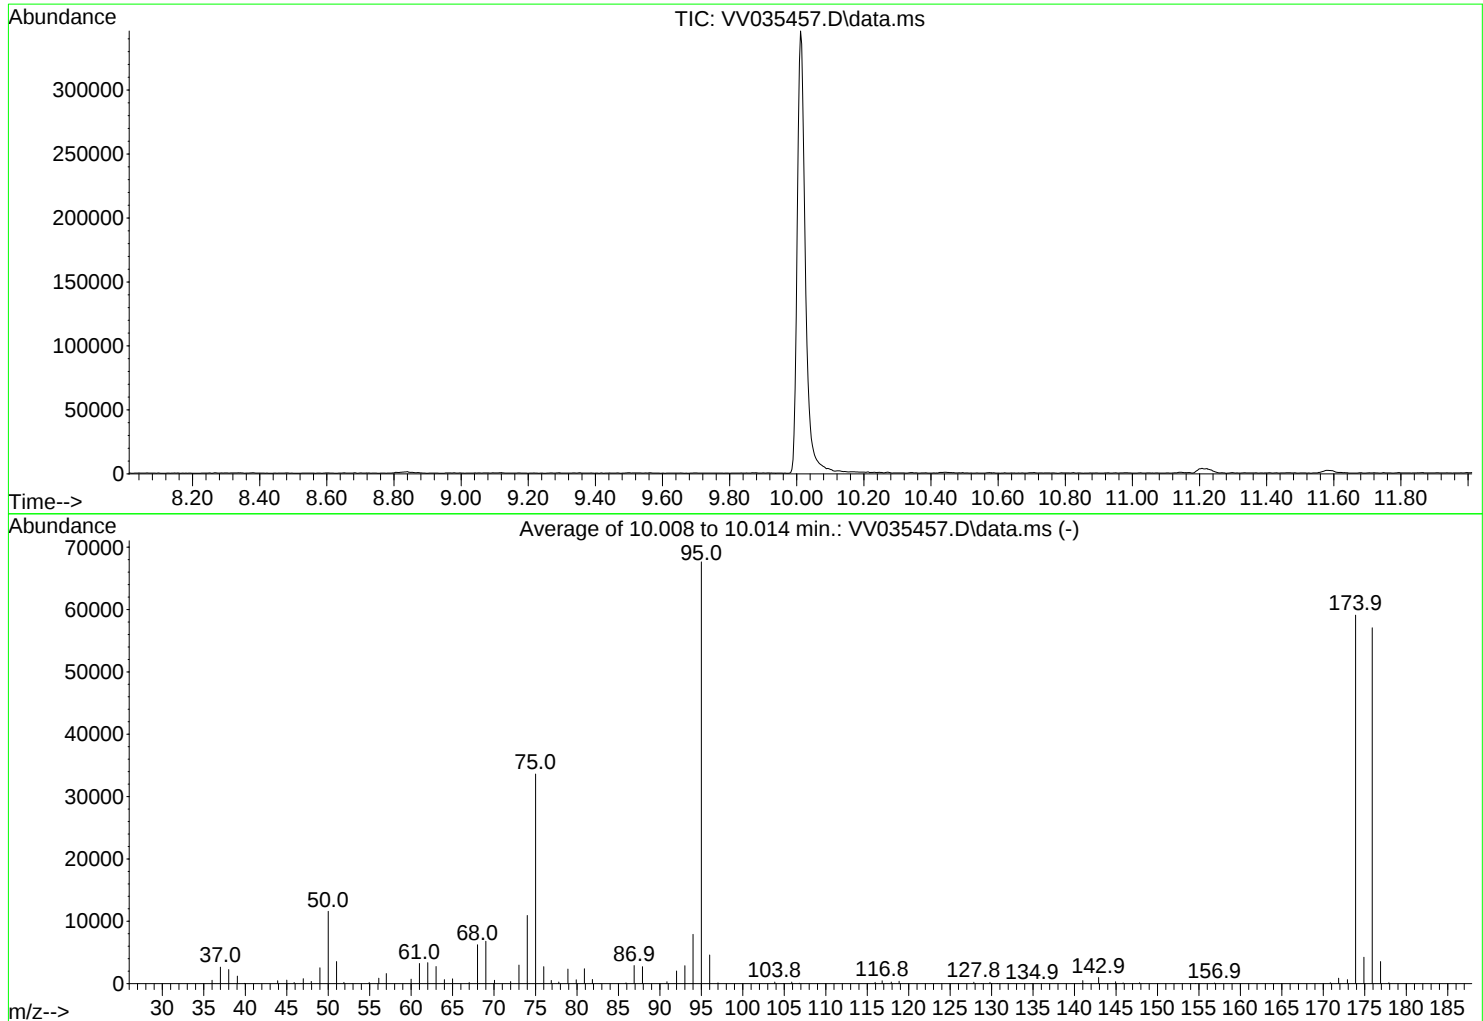

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	11592	PASS
75	95	30	80	49.7	33627	PASS
95	95	100	100	100.0	67648	PASS
96	95	5	9	6.8	4594	PASS
173	174	0.00	2	1.1	641	PASS
174	95	50	120	87.4	59104	PASS
175	174	5	9	7.2	4247	PASS
176	174	95	105	96.5	57061	PASS
177	176	5	10	6.2	3545	PASS

m/z	Abundance
40.00	199.0
43.90	334.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293

m/z	Abundance
36.00	559.0
37.00	2508.0
38.00	2227.0
39.10	1210.0
39.90	249.0
43.90	738.0
45.00	522.0
45.90	177.0
47.00	782.0
48.00	365.0
49.00	2557.0
50.00	11305.0
51.00	3494.0
51.90	167.0
54.90	156.0
56.10	816.0
57.00	1578.0
60.00	698.0
61.00	3224.0
62.00	3281.0
63.00	2682.0
64.00	641.0
65.00	674.0
67.00	183.0
68.00	6095.0
69.00	6521.0
70.00	501.0
72.00	291.0
73.00	2893.0
74.00	10598.0
75.00	32680.0
76.00	2815.0
76.90	463.0
77.80	267.0
78.90	2287.0
79.90	640.0
80.90	2320.0
81.90	658.0
82.80	116.0
86.00	142.0
86.90	2842.0
87.90	2441.0
90.90	273.0
92.00	1991.0
93.00	2832.0
94.00	7556.0
95.00	65272.0
96.00	4593.0
97.00	134.0
103.80	227.0
105.90	279.0
116.00	214.0
116.80	477.0
117.90	264.0
118.90	432.0
127.90	202.0
129.90	222.0
130.70	105.0
141.00	464.0
142.90	948.0
144.90	329.0
145.90	160.0
147.90	148.0
170.80	175.0
171.80	689.0
173.00	642.0
173.90	56192.0
174.90	4038.0
175.90	53800.0
176.90	3490.0
177.90	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293

m/z	Abundance
36.00	587.0
37.00	2727.0
38.00	2278.0
39.00	1240.0
39.90	289.0
43.90	827.0
45.00	569.0
45.90	186.0
47.00	835.0
48.00	356.0
49.00	2636.0
50.00	12029.0
51.00	3661.0
51.90	215.0
54.90	169.0
56.10	901.0
57.00	1672.0
60.00	750.0
61.00	3351.0
62.00	3495.0
63.00	2814.0
64.00	689.0
65.00	761.0
67.00	195.0
68.00	6475.0
69.00	7043.0
70.10	556.0
72.00	359.0
73.00	3082.0
74.00	11316.0
75.00	34880.0
76.00	2762.0
76.90	511.0
77.80	284.0
78.90	2378.0
79.90	624.0
80.90	2431.0
81.90	706.0
85.90	143.0
86.90	2982.0
87.90	2765.0
90.90	316.0
92.00	2109.0
93.00	2982.0
94.00	8119.0
95.00	70088.0
96.00	4709.0
97.00	130.0
103.90	277.0
104.90	106.0
105.90	261.0
106.80	108.0
115.90	224.0
116.80	489.0
117.90	264.0
118.90	384.0
127.80	230.0
128.80	107.0
129.80	200.0
141.00	489.0
142.90	1025.0
145.00	316.0
145.90	134.0
147.90	172.0
156.90	133.0
170.90	174.0
171.80	924.0
172.90	657.0
173.90	61056.0
174.90	4388.0
175.90	59240.0
176.90	3634.0
177.90	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293

m/z	Abundance
36.00	505.0
37.00	2680.0
38.00	2248.0
39.00	1208.0
39.90	254.0
43.90	838.0
45.00	596.0
45.90	162.0
47.00	741.0
47.90	329.0
49.00	2431.0
50.00	11441.0
51.00	3491.0
51.90	229.0
52.90	105.0
55.00	182.0
56.10	876.0
57.00	1626.0
60.00	707.0
61.00	3098.0
62.00	3286.0
63.00	2730.0
64.00	617.0
65.00	872.0
67.00	174.0
68.00	6143.0
69.00	6851.0
70.10	559.0
72.00	372.0
73.00	2972.0
74.00	10870.0
75.00	33320.0
76.00	2576.0
76.90	539.0
77.80	259.0
78.90	2321.0
79.90	594.0
80.90	2376.0
81.80	680.0
85.80	124.0
86.90	2915.0
87.90	2974.0
90.80	314.0
92.00	2007.0
93.00	2840.0
94.00	8041.0
95.00	67584.0
96.00	4480.0
97.00	120.0
103.90	282.0
105.90	218.0
106.80	113.0
115.90	203.0
116.80	428.0
117.90	243.0
118.80	336.0
127.80	251.0
129.70	212.0
134.90	108.0
141.00	504.0
142.90	1000.0
144.90	283.0
145.80	119.0
147.80	174.0
154.60	112.0
156.90	171.0
170.90	146.0
171.90	1049.0
172.80	623.0
173.90	60064.0
174.90	4316.0
175.90	58144.0
176.90	3512.0
177.90	159.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293