

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV043019\
 Data File : VV010557.D
 Acq On : 29 Apr 2019 19:47
 Operator : SY/MD
 Sample : K2590-20
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XE8

Quant Time: Apr 30 07:11:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Apr 30 06:45:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	218485	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	206656	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	93178	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	46375	4.36	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.20%
7) Chloroethane-d5	1.58	69	25630	4.51	ug/L	0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.20%
11) 1,1-Dichloroethene-d2	2.13	63	68930	3.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.00%
20) 2-Butanone-d5	3.95	46	123683	45.12	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	90.24%
24) Chloroform-d	4.40	84	140650	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
26) 1,2-Dichloroethane-d4	5.08	65	66746	5.08	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.60%
32) Benzene-d6	5.10	84	275116	5.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.80%
36) 1,2-Dichloropropane-d6	6.12	67	74055	5.09	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.80%
41) Toluene-d8	7.36	98	244027	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.20%
43) trans-1,3-Dichloropropene-	7.67	79	26534	4.77	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.40%
46) 2-Hexanone-d5	8.14	63	105698	45.06	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.12%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	55647	4.82	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	101180	5.63	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.60%


Target Compounds					Ovalue
13) Acetone	2.21	43	6912	5.062 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV043019\
Data File : VV010557.D
Acq On : 29 Apr 2019 19:47
Operator : SY/MD
Sample : K2590-20
Misc : 25mL/MSVOA V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XE8

Quant Time: Apr 30 07:11:52 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Apr 30 06:45:30 2019
Response via : Initial Calibration

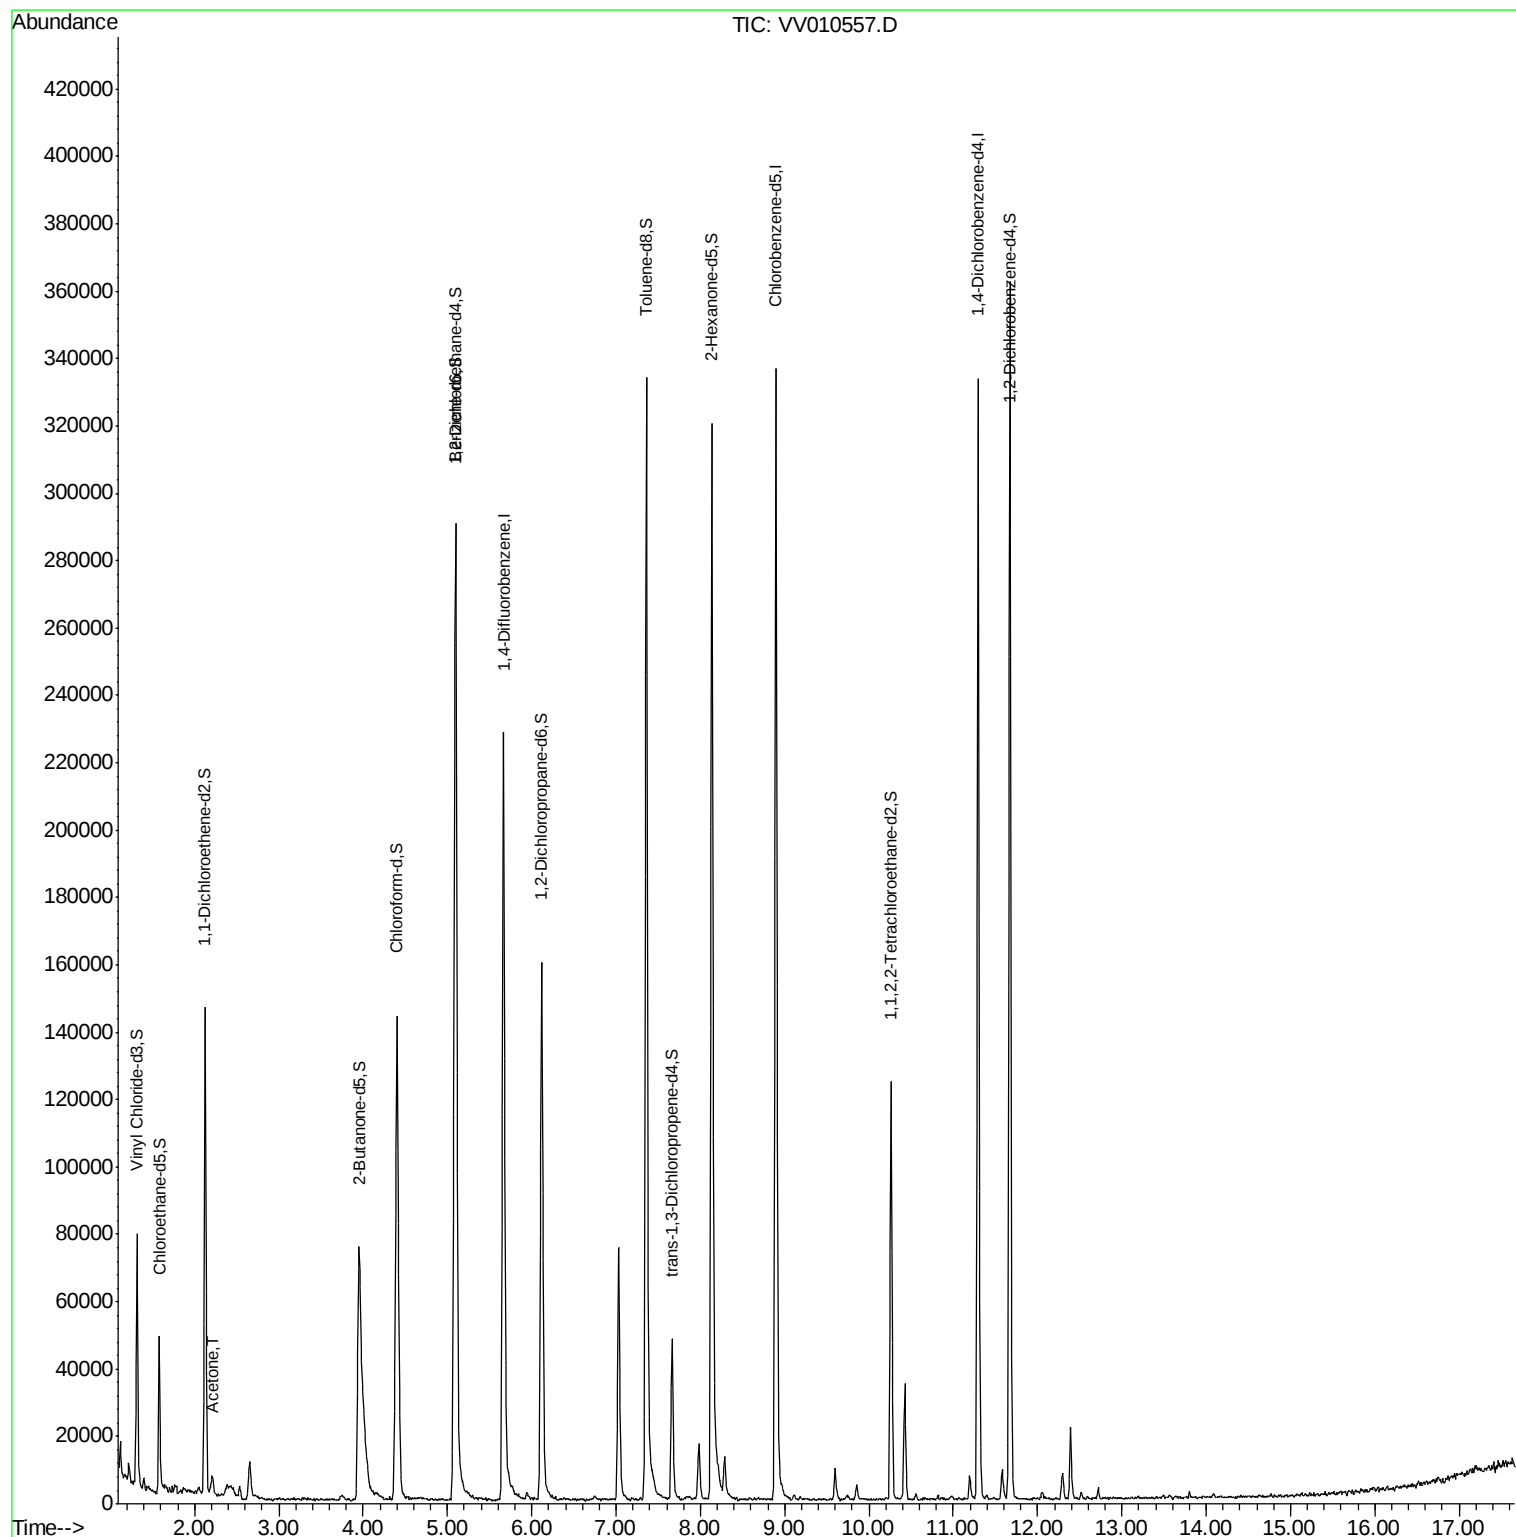

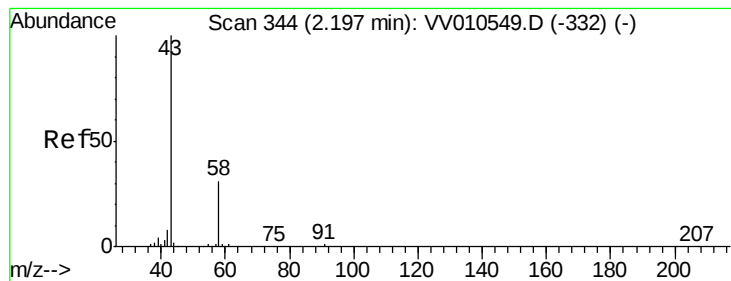

#13

Acetone

Concen: 5.062 ug/L

RT: 2.21 min Scan# 349

Delta R.T. 0.02 min

Lab File: VV010557.D

Acq: 29 Apr 2019 19:47


Instrument :
MSVOA_V
ClientSampleId :
C0XE8

Tot Ion: 43 Resp: 6912

Ion Ratio Lower Upper

43 100

58 30.5 0.0 57.4

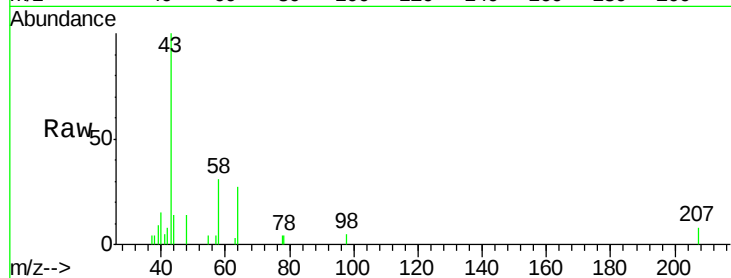

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

