

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV043019\
 Data File : VV010559.D
 Acq On : 29 Apr 2019 20:37
 Operator : SY/MD
 Sample : K2593-07
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XE4

Quant Time: Apr 30 07:16:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Apr 30 06:45:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	226063	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	218441	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	98361	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	45861	4.17	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.40%
7) Chloroethane-d5	1.58	69	26598	4.52	ug/L	0.01
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.40%
11) 1,1-Dichloroethene-d2	2.13	63	66017	3.19	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.80%
20) 2-Butanone-d5	3.96	46	125486	44.25	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.50%
24) Chloroform-d	4.40	84	140642	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.40%
26) 1,2-Dichloroethane-d4	5.08	65	66980	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.60%
32) Benzene-d6	5.10	84	264338	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.12	67	75081	4.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.60%
41) Toluene-d8	7.36	98	242989	4.72	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.40%
43) trans-1,3-Dichloropropene-	7.67	79	24401	4.15	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.00%
46) 2-Hexanone-d5	8.14	63	107115	43.20	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.40%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	55548	4.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	102473	5.40	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.00%


Target Compounds					Ovalue
13) Acetone	2.21	43	6478	4.585 ug/L	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV043019\
Data File : VV010559.D
Acq On : 29 Apr 2019 20:37
Operator : SY/MD
Sample : K2593-07
Misc : 25mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XE4

Quant Time: Apr 30 07:16:17 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Apr 30 06:45:30 2019
Response via : Initial Calibration

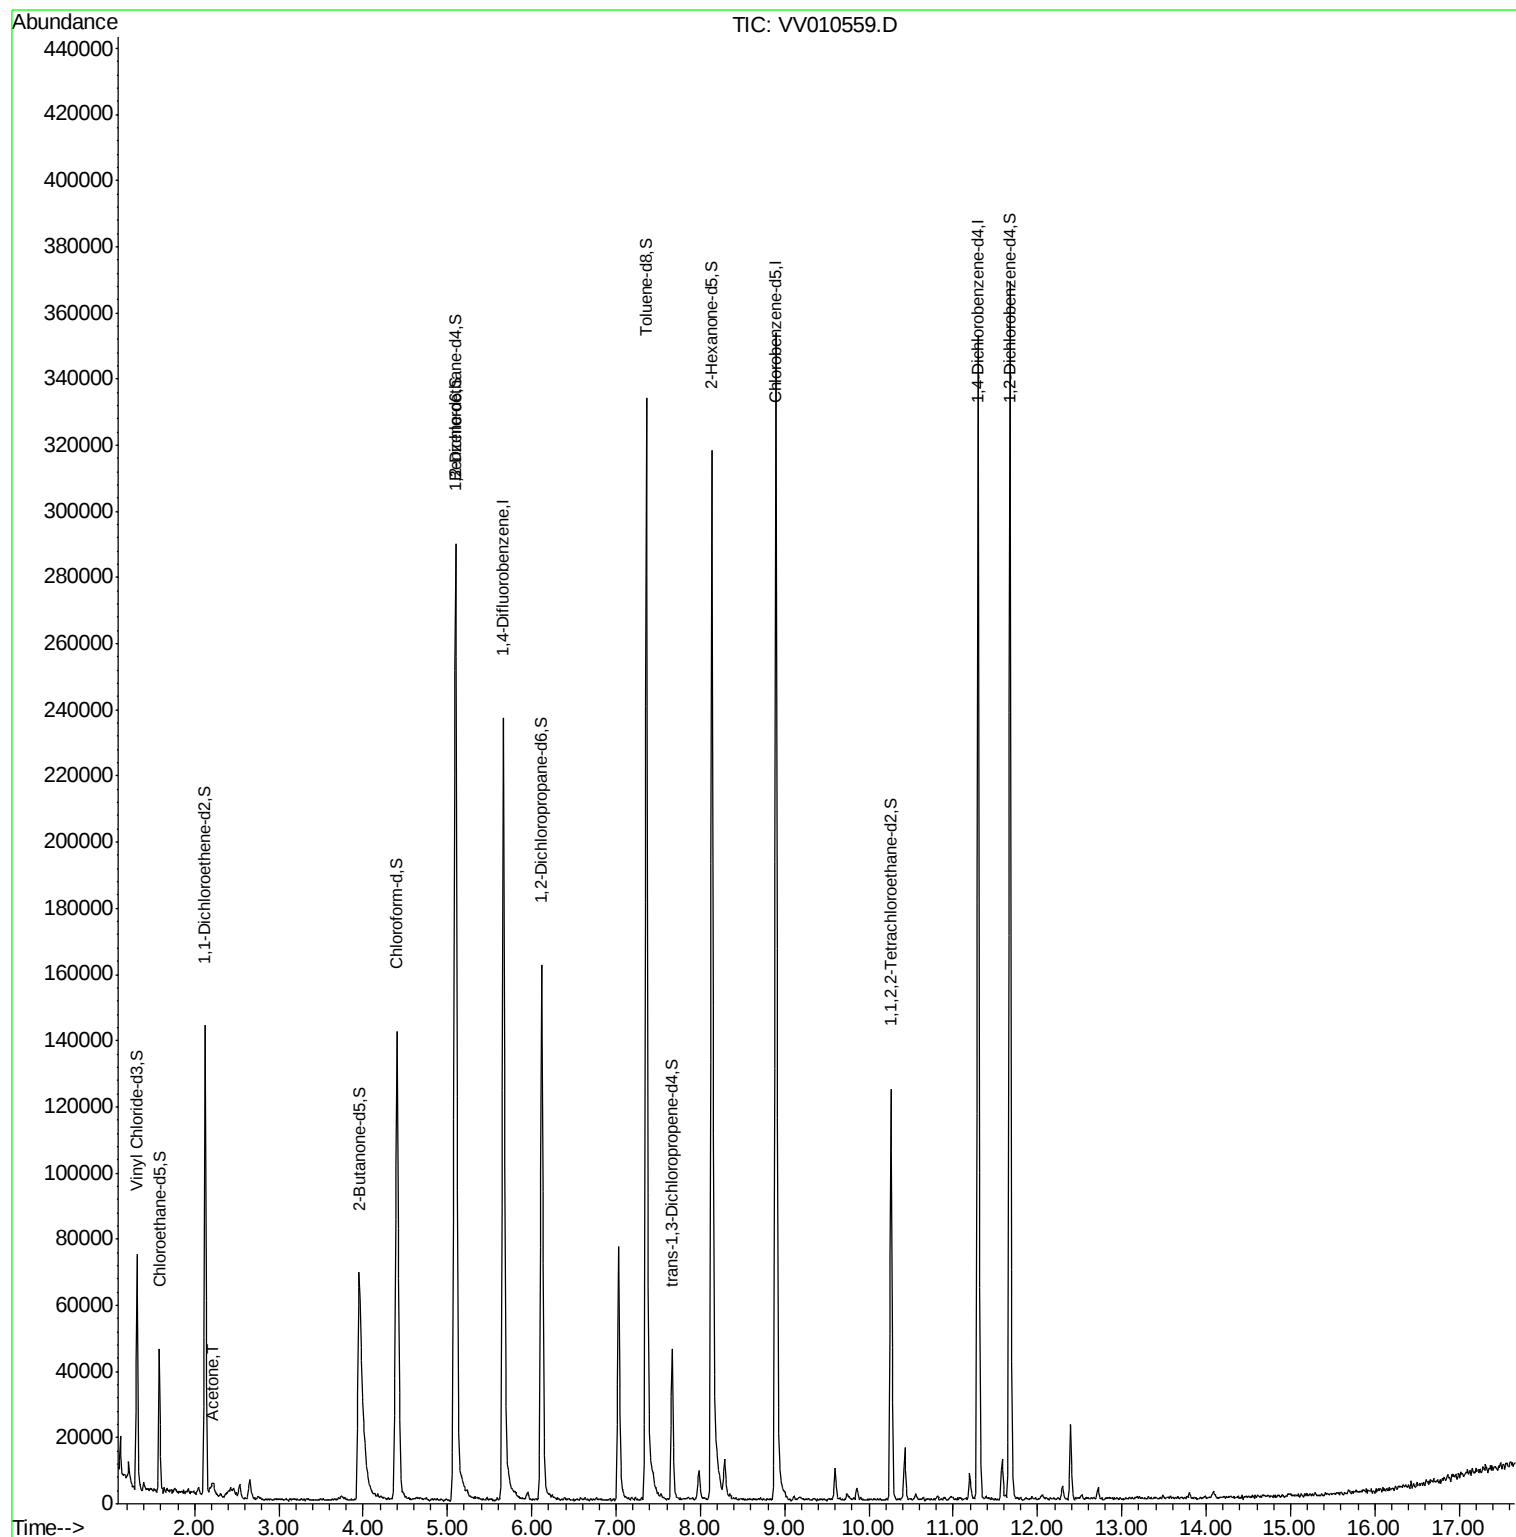

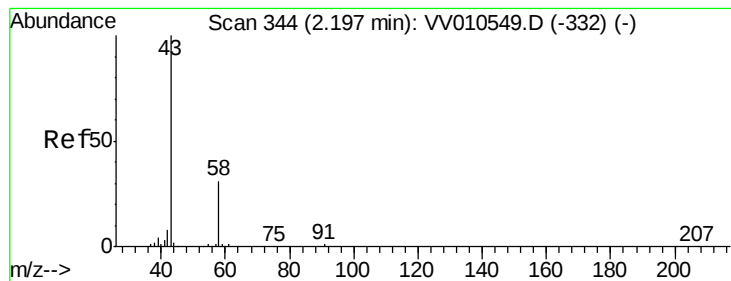

#13
 Acetone
 Concen: 4.585 ug/L
 RT: 2.21 min Scan# 348
 Delta R.T. 0.01 min
 Lab File: VV010559.D
 Acq: 29 Apr 2019 20:37

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XE4

Tot Ion: 43 Resp: 6478
 Ion Ratio Lower Upper
 43 100
 58 9.0 0.0 57.4

