

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV043019\
 Data File : VV010560.D
 Acq On : 29 Apr 2019 21:03
 Operator : SY/MD
 Sample : K2593-20
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XG9

Quant Time: Apr 30 07:19:36 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Apr 30 06:45:30 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	217860	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	220583	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	100343	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	47106	4.44	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.80%
7) Chloroethane-d5	1.57	69	33161	5.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	117.00%
11) 1,1-Dichloroethene-d2	2.13	63	62388	3.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.60%
20) 2-Butanone-d5	3.94	46	125214	45.81	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	91.62%
24) Chloroform-d	4.40	84	125730	4.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.40%
26) 1,2-Dichloroethane-d4	5.08	65	65361	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.80%
32) Benzene-d6	5.10	84	245881	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
36) 1,2-Dichloropropane-d6	6.12	67	70553	4.55	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.00%
41) Toluene-d8	7.36	98	233362	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.60%
43) trans-1,3-Dichloropropene-	7.67	79	25458	4.29	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.80%
46) 2-Hexanone-d5	8.13	63	107922	43.10	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.20%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	54800	4.45	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	101512	5.25	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.00%


Target Compounds					Ovalue
13) Acetone	2.19	43	3420	2.512 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV043019\
Data File : VV010560.D
Acq On : 29 Apr 2019 21:03
Operator : SY/MD
Sample : K2593-20
Misc : 25mL/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0XG9

Quant Time: Apr 30 07:19:36 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Apr 30 06:45:30 2019
Response via : Initial Calibration

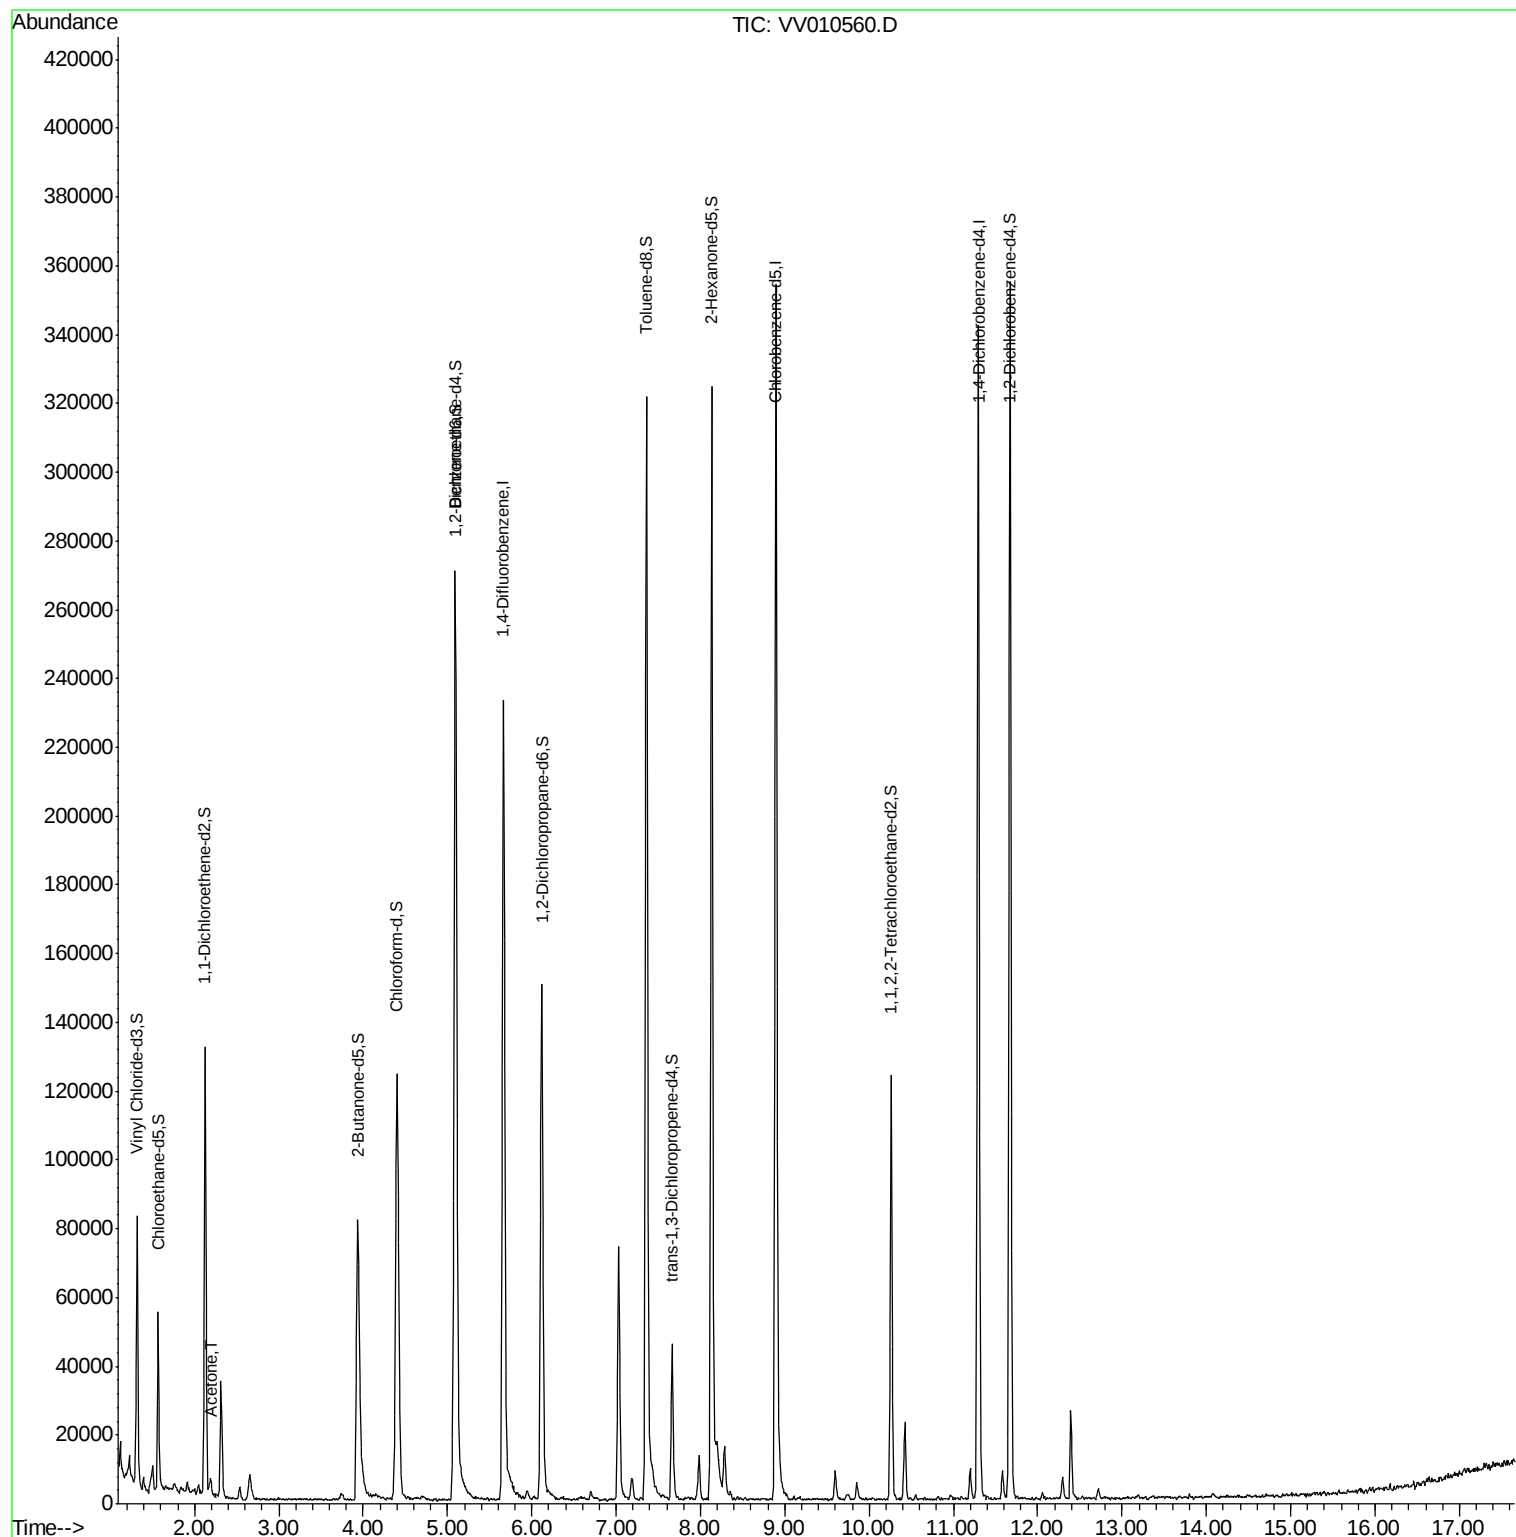

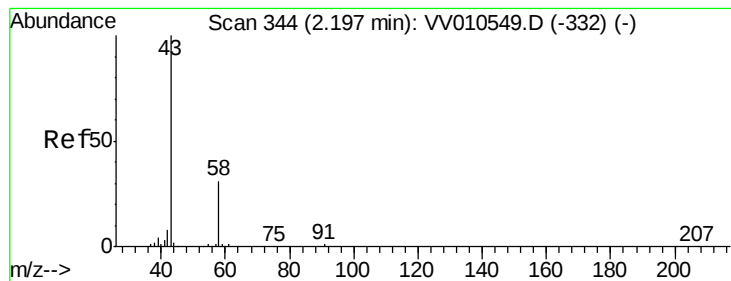

#13
 Acetone
 Concen: 2.512 ug/L
 RT: 2.19 min Scan# 343
 Delta R.T. -0.00 min
 Lab File: VV010560.D
 Acq: 29 Apr 2019 21:03

Instrument :
 MSVOA_V
 ClientSampleId :
 C0XG9

Tot Ion: 43 Resp: 3420
 Ion Ratio Lower Upper
 43 100
 58 25.1 0.0 57.4

