


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV043019\
Data File : VV010548.D
Acq On : 29 Apr 2019 15:08
Operator : SY/MD
Sample : BFB39
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB39

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Tue Apr 30 06:45:30 2019

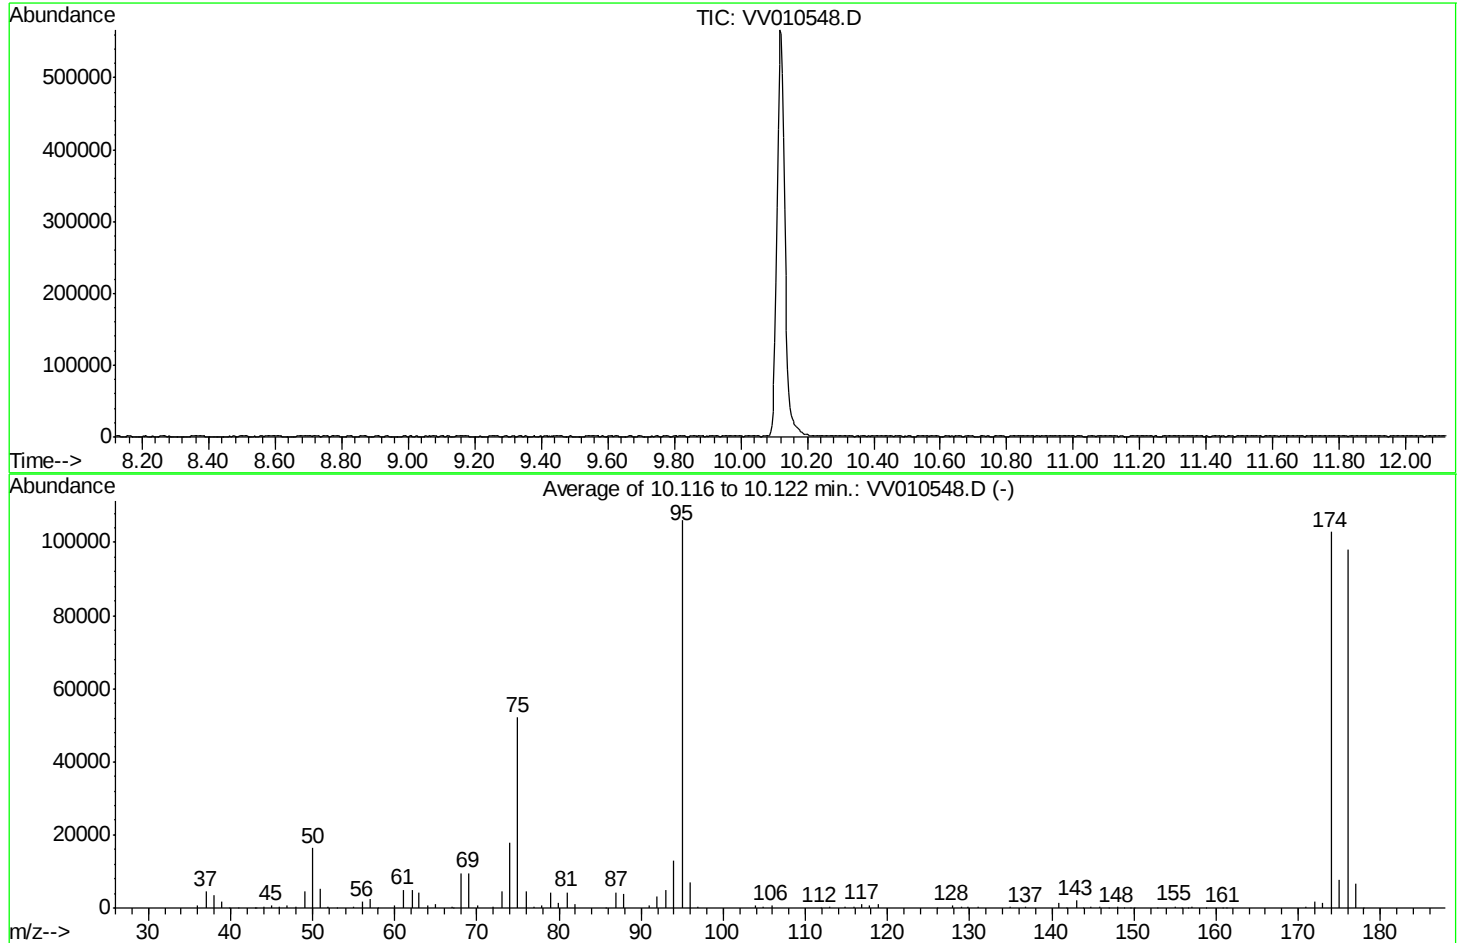

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	16299	PASS
75	95	30	80	49.1	52032	PASS
95	95	100	100	100.0	106050	PASS
96	95	5	9	6.6	7027	PASS
173	174	0.00	2	1.5	1550	PASS
174	95	50	120	97.1	102944	PASS
175	174	5	9	7.6	7845	PASS
176	174	95	101	95.4	98181	PASS
177	176	5	9	6.8	6708	PASS

m/z	Abundance
36.00	530.0
37.00	4201.0
38.00	3174.0
39.00	1654.0
39.90	828.0
40.90	109.0
43.00	105.0
44.00	771.0
44.90	672.0
46.00	251.0
46.90	869.0
47.90	440.0
49.00	4338.0
50.00	15666.0
51.00	5215.0
51.80	235.0
55.00	367.0
56.00	1508.0
57.00	2386.0
57.90	121.0
60.00	801.0
61.00	5328.0
62.10	4689.0
63.00	3782.0
64.00	583.0
65.00	1021.0
66.90	466.0
68.00	9074.0
69.00	8773.0
70.00	726.0
71.90	472.0
73.00	4670.0
74.00	17184.0
75.00	50152.0
76.00	4421.0
76.90	426.0
78.00	563.0
78.90	3973.0
79.90	1430.0
81.00	4432.0
82.00	1051.0
85.80	226.0
87.00	4187.0
87.90	3579.0
91.00	608.0
91.90	2942.0
93.00	4217.0
94.00	12723.0
95.00	100256.0
96.00	6800.0
96.90	230.0
103.90	498.0
104.80	268.0
105.90	693.0
113.00	229.0
114.80	179.0
115.90	436.0
116.90	881.0
117.90	516.0
118.90	1025.0
127.90	735.0
129.00	249.0
129.80	489.0
131.00	259.0
134.80	152.0
136.80	279.0
140.90	1280.0
141.70	187.0
142.90	2036.0
143.80	202.0
144.70	335.0
145.90	225.0
146.90	113.0
147.90	302.0
148.80	117.0
149.50	122.0
150.10	189.0
155.00	462.0
157.00	175.0
158.70	223.0
160.80	115.0
170.90	258.0
172.00	1591.0
173.00	1480.0
174.00	94824.0
175.00	7347.0
176.00	90320.0
177.00	6323.0
177.90	146.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
36.00	610.0
37.00	4612.0
38.00	3575.0
39.00	1872.0
39.90	698.0
40.90	126.0
43.20	135.0
44.00	744.0
45.00	588.0
46.00	259.0
46.90	937.0
47.90	427.0
49.00	4632.0
50.00	16800.0
51.00	5396.0
51.80	199.0
53.00	144.0
55.10	338.0
56.00	1713.0
57.00	2456.0
58.00	196.0
60.00	781.0
61.00	5126.0
62.10	5047.0
63.00	4226.0
64.10	611.0
65.00	953.0
66.90	385.0
68.00	9833.0
69.00	10002.0
70.10	828.0
71.90	540.0
73.00	4629.0
74.00	18096.0
75.00	53800.0
76.00	4416.0
76.90	520.0
77.90	572.0
78.90	4440.0
79.90	1484.0
81.00	4430.0
82.00	1088.0
85.70	215.0
87.00	4445.0
87.90	4129.0
91.00	582.0
91.90	3288.0
93.00	5010.0
94.00	13295.0
95.00	109536.0
96.00	7308.0
96.90	219.0
103.90	585.0
104.80	270.0
105.90	719.0
111.80	139.0
113.00	208.0
114.80	253.0
115.80	448.0
116.90	1038.0
117.80	598.0
118.90	905.0
127.90	719.0
128.90	276.0
129.80	468.0
131.00	311.0
134.90	184.0
136.80	355.0
140.90	1385.0
143.00	2113.0
144.70	417.0
145.90	272.0
148.00	339.0
148.70	110.0
149.50	104.0
150.10	177.0
155.00	509.0
155.80	124.0
156.60	183.0
157.00	219.0
158.70	181.0
160.80	124.0
171.00	259.0
172.00	1952.0
173.00	1588.0
174.00	106296.0
175.00	8165.0
176.00	101312.0
177.00	6939.0
177.90	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
36.00	665.0
37.00	4400.0
38.00	3675.0
39.00	1934.0
39.90	644.0
43.20	164.0
43.90	686.0
45.00	567.0
45.90	250.0
47.00	790.0
47.90	440.0
49.00	4292.0
50.00	16432.0
51.00	5174.0
51.90	220.0
53.00	207.0
55.00	271.0
56.00	1652.0
57.00	2485.0
58.00	236.0
60.00	741.0
61.00	4501.0
62.10	4820.0
63.00	4244.0
64.00	633.0
65.00	854.0
67.10	307.0
68.00	9512.0
69.00	10061.0
70.10	852.0
71.90	561.0
73.00	4537.0
74.00	17808.0
75.00	52144.0
76.00	4331.0
76.90	565.0
77.90	489.0
78.90	4444.0
80.00	1418.0
81.00	4088.0
81.90	1038.0
85.70	111.0
86.90	4225.0
87.90	4108.0
91.00	484.0
92.00	3157.0
93.00	5173.0
94.00	13016.0
95.00	108360.0
96.00	6974.0
97.00	241.0
103.90	624.0
104.80	227.0
105.90	592.0
111.80	123.0
113.00	164.0
114.90	294.0
115.80	434.0
116.90	1019.0
117.70	573.0
118.90	754.0
126.00	111.0
127.90	564.0
128.90	293.0
129.90	463.0
131.00	258.0
134.90	257.0
136.80	356.0
140.90	1438.0
143.00	2113.0
143.70	199.0
144.70	468.0
145.80	267.0
148.00	333.0
150.10	125.0
152.90	120.0
154.90	473.0
155.80	144.0
157.10	244.0
158.70	129.0
160.80	103.0
161.20	136.0
171.00	211.0
172.00	1933.0
173.00	1584.0
174.00	107712.0
175.00	8024.0
176.00	102912.0
177.00	6864.0
177.90	183.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

Scan 2794 (10.074 min): VV010548.D
BFB39

m/z	Abundance
39.80	613.0
44.10	401.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39