

Quantitation Report (QT/LSC Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV043020\
 Data File : VV015844.D
 Acq On : 30 Apr 2020 19:19
 Operator : SY/MD
 Sample : L2431-17
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :
 ETKS6

Quant Time: Mav 02 05:15:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 01 01:42:43 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 5/4/2020 12:34:51 PM

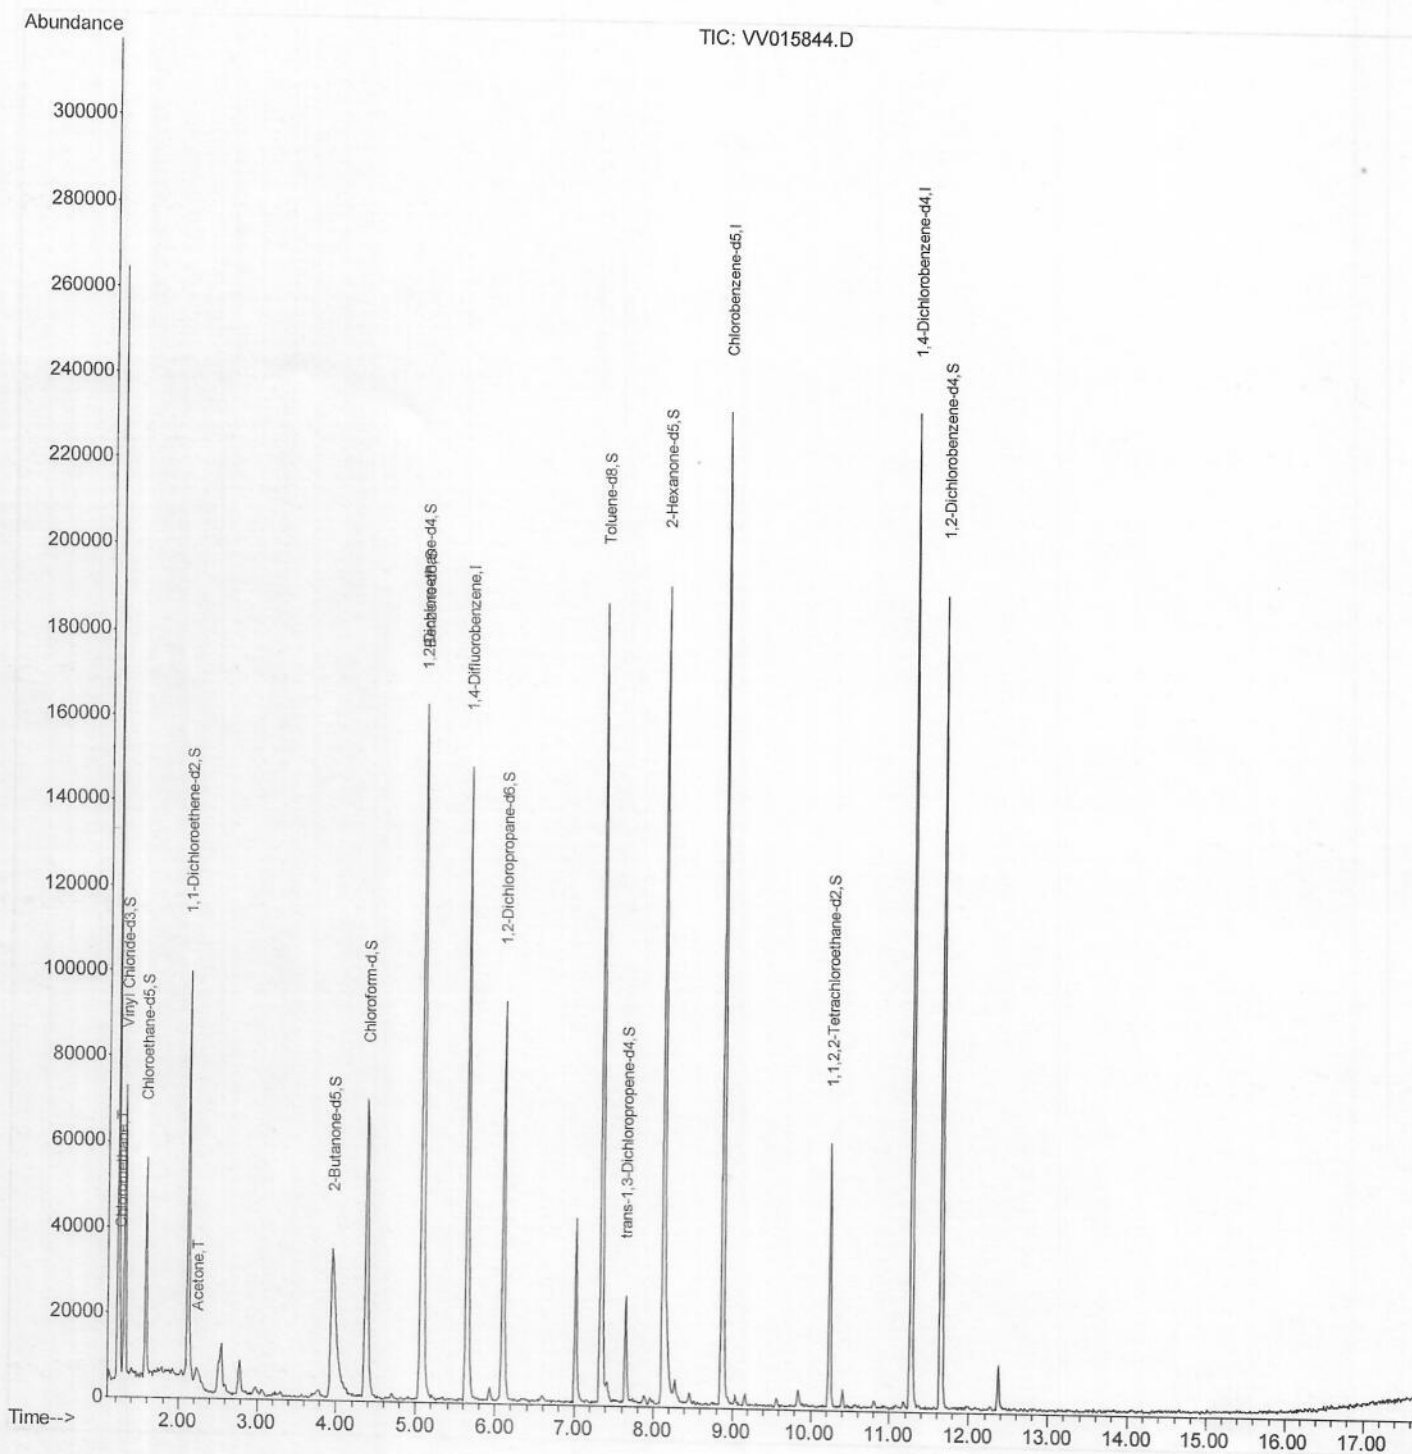

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV043020\
 Data File : VV015844.D
 Acq On : 30 Apr 2020 19:19
 Operator : SY/MD
 Sample : L2431-17
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKS6

Manual Integrations
 APPROVED

apatel
 5/4/2020 12:34:51 PM

Quant Time: May 01 01:48:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 01 01:42:43 2020
 Response via : Initial Calibration

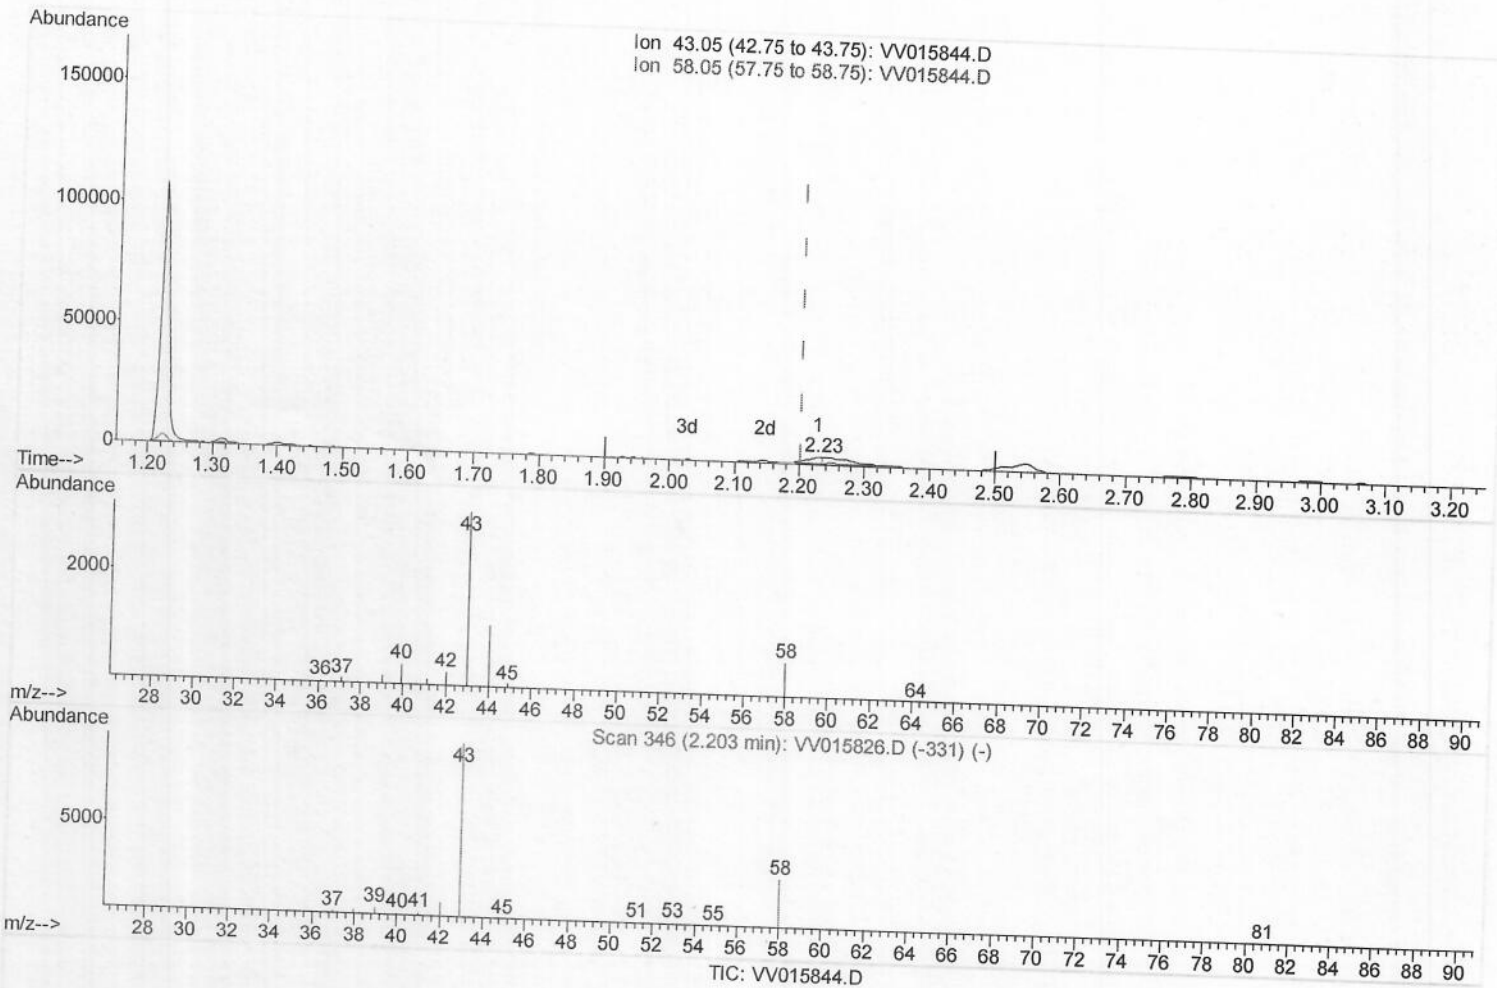

(13) Acetone (T)

2.228min (+0.026) 3.75ug/L

response 5120

Ion	Exp%	Act%
43.05	100	100
58.05	28.80	34.36
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV043020\
 Data File : VV015844.D
 Acq On : 30 Apr 2020 19:19
 Operator : SY/MD
 Sample : L2431-17
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETKS6

Manual Integrations
 APPROVED

apatel
 5/4/2020 12:34:51 PM

Quant Time: Mav 01 01:48:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 01 01:42:43 2020
 Response via : Initial Calibration

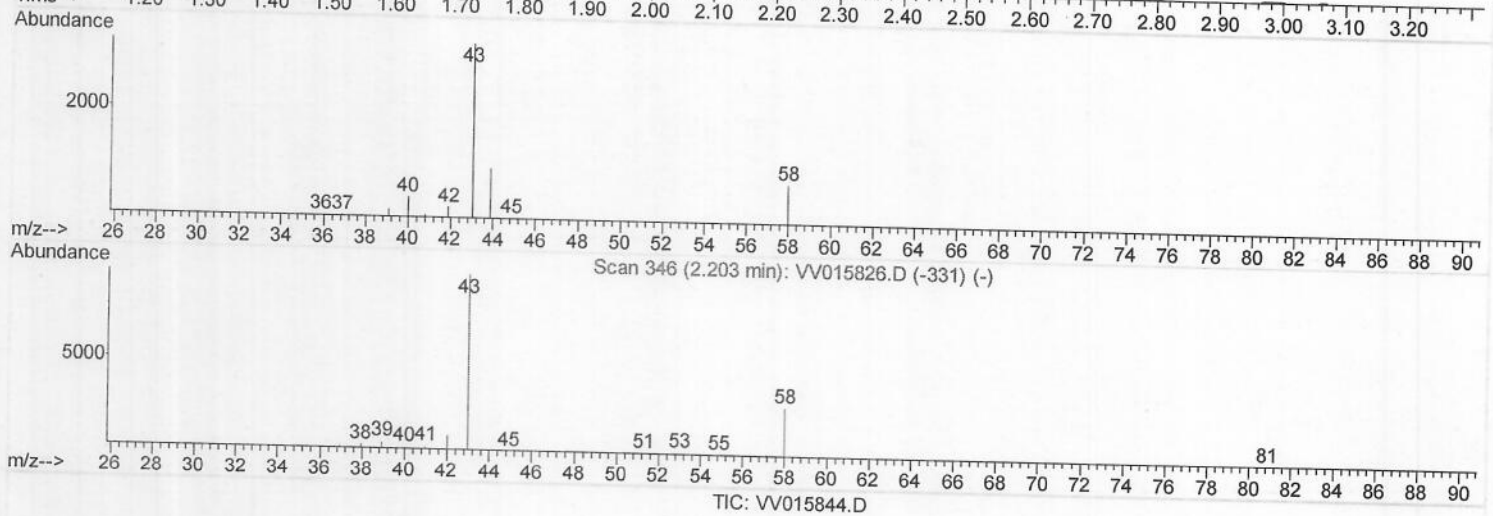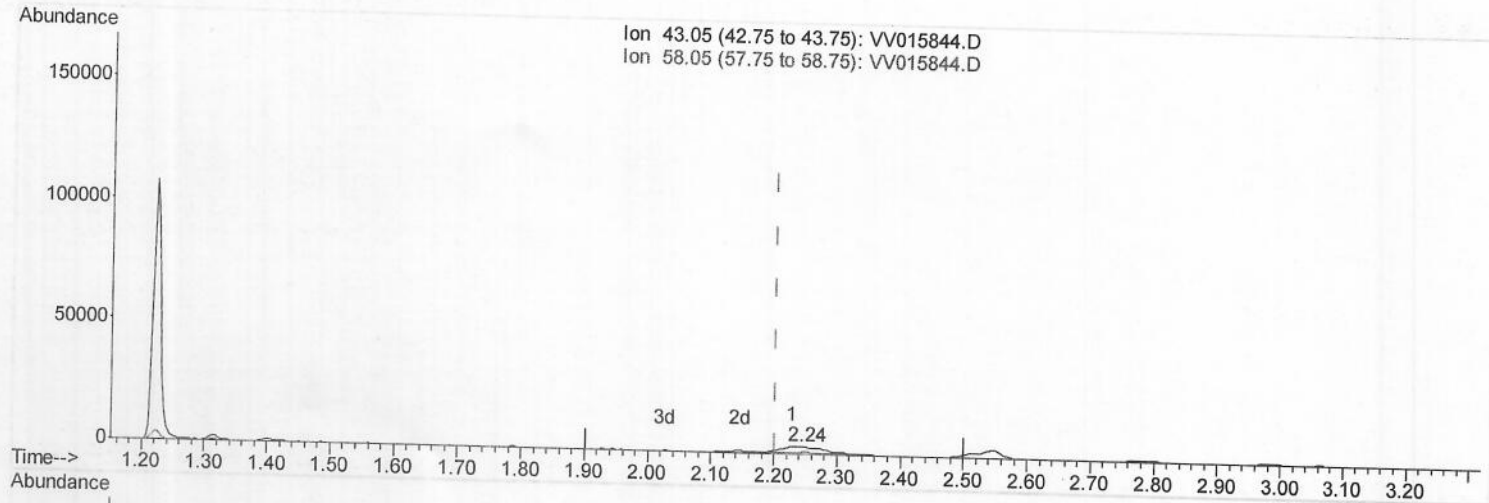

(13) Acetone (T)

2.245min (+0.042) 11.46ug/L m

response 15636

Ion	Exp%	Act%
43.05	100	100
58.05	28.80	11.25
0.00	0.00	0.00
0.00	0.00	0.00

MD
 05/5/2020

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV043020\
 Data File : VV015844.D
 Acq On : 30 Apr 2020 19:19
 Operator : SY/MD
 Sample : L2431-17
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 ETKS6

Manual Integrations
 APPROVED

apatel
 5/4/2020 12:34:51 PM

Quant Time: May 02 05:15:58 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 01 01:42:43 2020
 Response via : Initial Calibration

Internal Standards		R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene		5.64	114	117113	5.00	ug/L	0.00
28) Chlorobenzene-d5		8.87	117	114452	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4		11.27	152	52622	5.00	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.31	65	34121	5.58	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.60%	
7) Chloroethane-d5		1.58	69	31517	5.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.80%	
11) 1,1-Dichloroethene-d2		2.12	63	52322	3.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	78.20%	
20) 2-Butanone-d5		3.95	46	96567	49.14	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.28%	
24) Chloroform-d		4.38	84	69864	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%	
26) 1,2-Dichloroethane-d4		5.06	65	40985	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.80%	
32) Benzene-d6		5.08	84	133968	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%	
36) 1,2-Dichloropropane-d6		6.10	67	41282	4.73	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.60%	
41) Toluene-d8		7.34	98	117811	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.80%	
43) trans-1,3-Dichloropropene-		7.65	79	13801	4.09	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.80%	
46) 2-Hexanone-d5		8.12	63	62672	38.07	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.14%	
57) 1,1,2,2-Tetrachloroethane-		10.24	84	27275	4.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.00%	
64) 1,2-Dichlorobenzene-d4		11.65	152	43423	4.85	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.00%	
Target Compounds							
3) Chloromethane		1.25	50	11122	1.282	ug/L	Ovalue 100
13) Acetone		2.24	43	15636m	11.458	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD
 05/3/2020