

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV043020\
 Data File : VV015827.D
 Acq On : 30 Apr 2020 11:15
 Operator : SY/MD
 Sample : VV0430WBL01
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK51

Quant Time: May 01 02:06:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 01 01:42:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	130052	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	125829	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	58816	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	36035	5.30	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.00%
7) Chloroethane-d5	1.58	69	32265	4.93	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.60%
11) 1,1-Dichloroethene-d2	2.12	63	53756	3.61	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.20%
20) 2-Butanone-d5	3.96	46	96045	44.01	ug/L	0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	88.02%
24) Chloroform-d	4.38	84	66501	4.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.00%
26) 1,2-Dichloroethane-d4	5.06	65	41509	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.60%
32) Benzene-d6	5.08	84	141315	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
36) 1,2-Dichloropropane-d6	6.10	67	44398	4.63	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.60%
41) Toluene-d8	7.34	98	126290	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.60%
43) trans-1,3-Dichloropropene-	7.65	79	14991	4.04	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.80%
46) 2-Hexanone-d5	8.12	63	68923	38.09	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	76.18%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	29210	4.09	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	81.80%
64) 1,2-Dichlorobenzene-d4	11.65	152	45013	4.50	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.00%


Target Compounds					Ovalue
25) Chloroform	4.41	83	6885	0.390 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV043020\
Data File : VV015827.D
Acq On : 30 Apr 2020 11:15
Operator : SY/MD
Sample : VV0430WBL01
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK51

Quant Time: May 01 02:06:24 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 01 01:42:43 2020
Response via : Initial Calibration

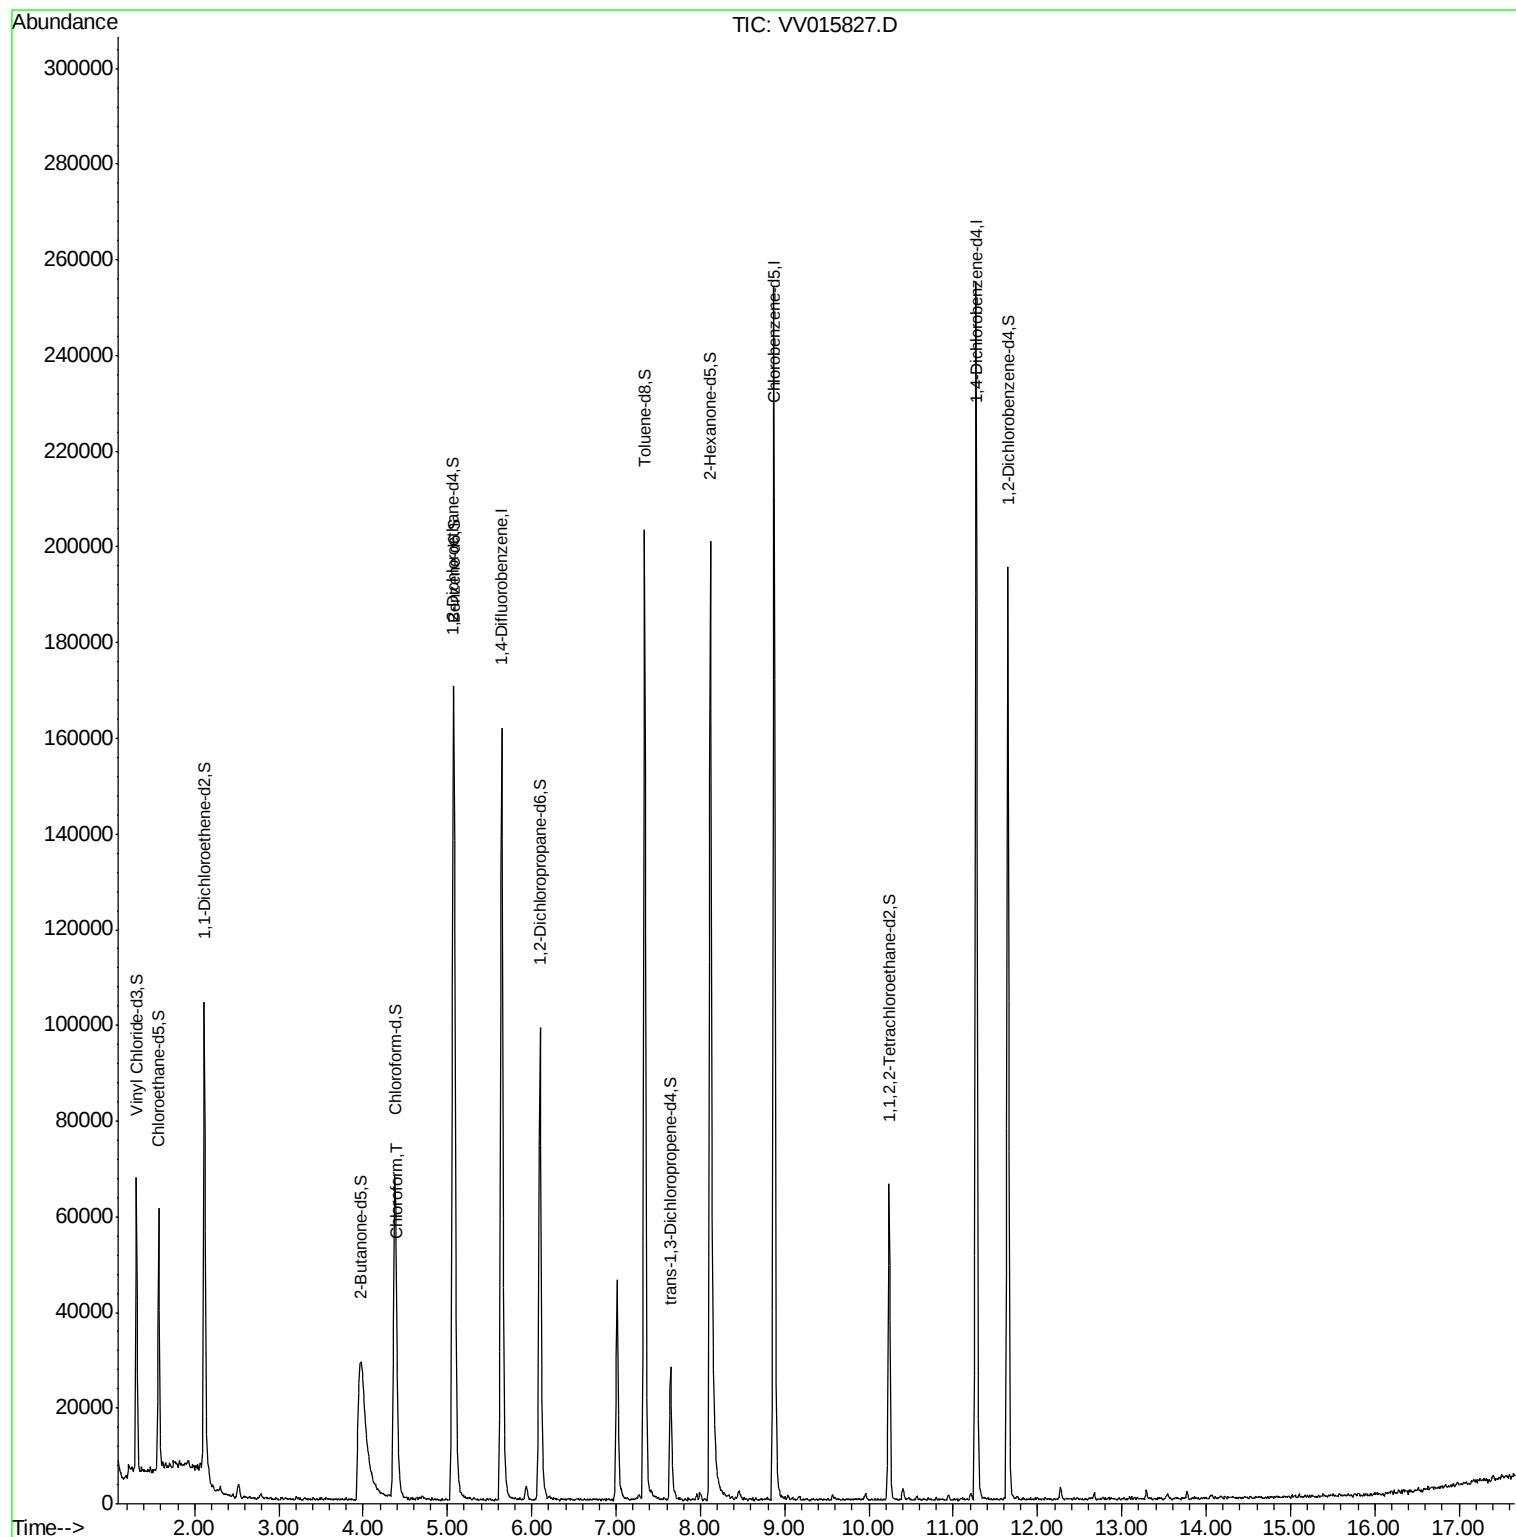

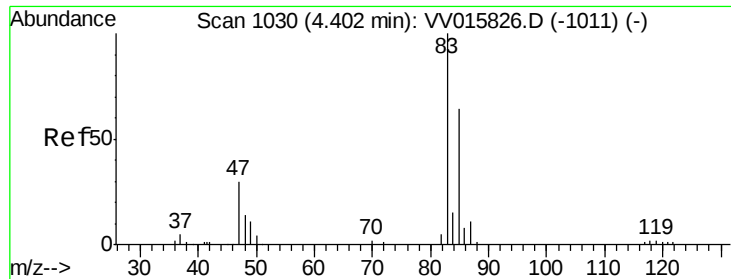

#25
 Chloroform
 Concen: 0.390 ug/L
 RT: 4.41 min Scan# 1031
 Delta R.T. 0.00 min
 Lab File: VV015827.D
 Acq: 30 Apr 2020 11:15

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK51

Tot Ion: 83 Resp: 6885
 Ion Ratio Lower Upper
 83 100
 85 64.5 46.1 85.5

