

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV043020\
 Data File : VV015828.D
 Acq On : 30 Apr 2020 11:48
 Operator : SY/MD
 Sample : L2421-09DL 100X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFSB0DL

Quant Time: May 01 02:11:55 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 01 01:42:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	134116	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	128083	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	62022	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	38467	5.49	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.80%
7) Chloroethane-d5	1.57	69	35206	5.21	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.20%
11) 1,1-Dichloroethene-d2	2.11	63	57932	3.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.60%
20) 2-Butanone-d5	3.96	46	98061	43.57	ug/L	0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	87.14%
24) Chloroform-d	4.37	84	69736	4.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.40%
26) 1,2-Dichloroethane-d4	5.06	65	44183	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.07	84	150117	4.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.20%
36) 1,2-Dichloropropane-d6	6.09	67	45565	4.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.20%
41) Toluene-d8	7.34	98	133916	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.20%
43) trans-1,3-Dichloropropene-	7.64	79	16069	4.25	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.00%
46) 2-Hexanone-d5	8.12	63	73243	39.76	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.52%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	30817	4.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.80%
64) 1,2-Dichlorobenzene-d4	11.65	152	47391	4.50	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.00%

Target Compounds


					Ovalue
5) Vinyl chloride	1.32	62	3710	0.350 ug/L	# 68
19) 1,1-Dichloroethane	3.21	63	5221	0.304 ug/L	96
22) cis-1,2-Dichloroethene	3.93	96	100119	10.360 ug/L	95
25) Chloroform	4.40	83	8817	0.484 ug/L	100
29) 1,1,1-Trichloroethane	4.63	97	7160	0.441 ug/L	97
34) Trichloroethene	5.94	95	136574	13.514 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV043020\
Data File : VV015828.D
Acq On : 30 Apr 2020 11:48
Operator : SY/MD
Sample : L2421-09DL 100X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFSB0DL

Quant Time: May 01 02:11:55 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 01 01:42:43 2020
Response via : Initial Calibration

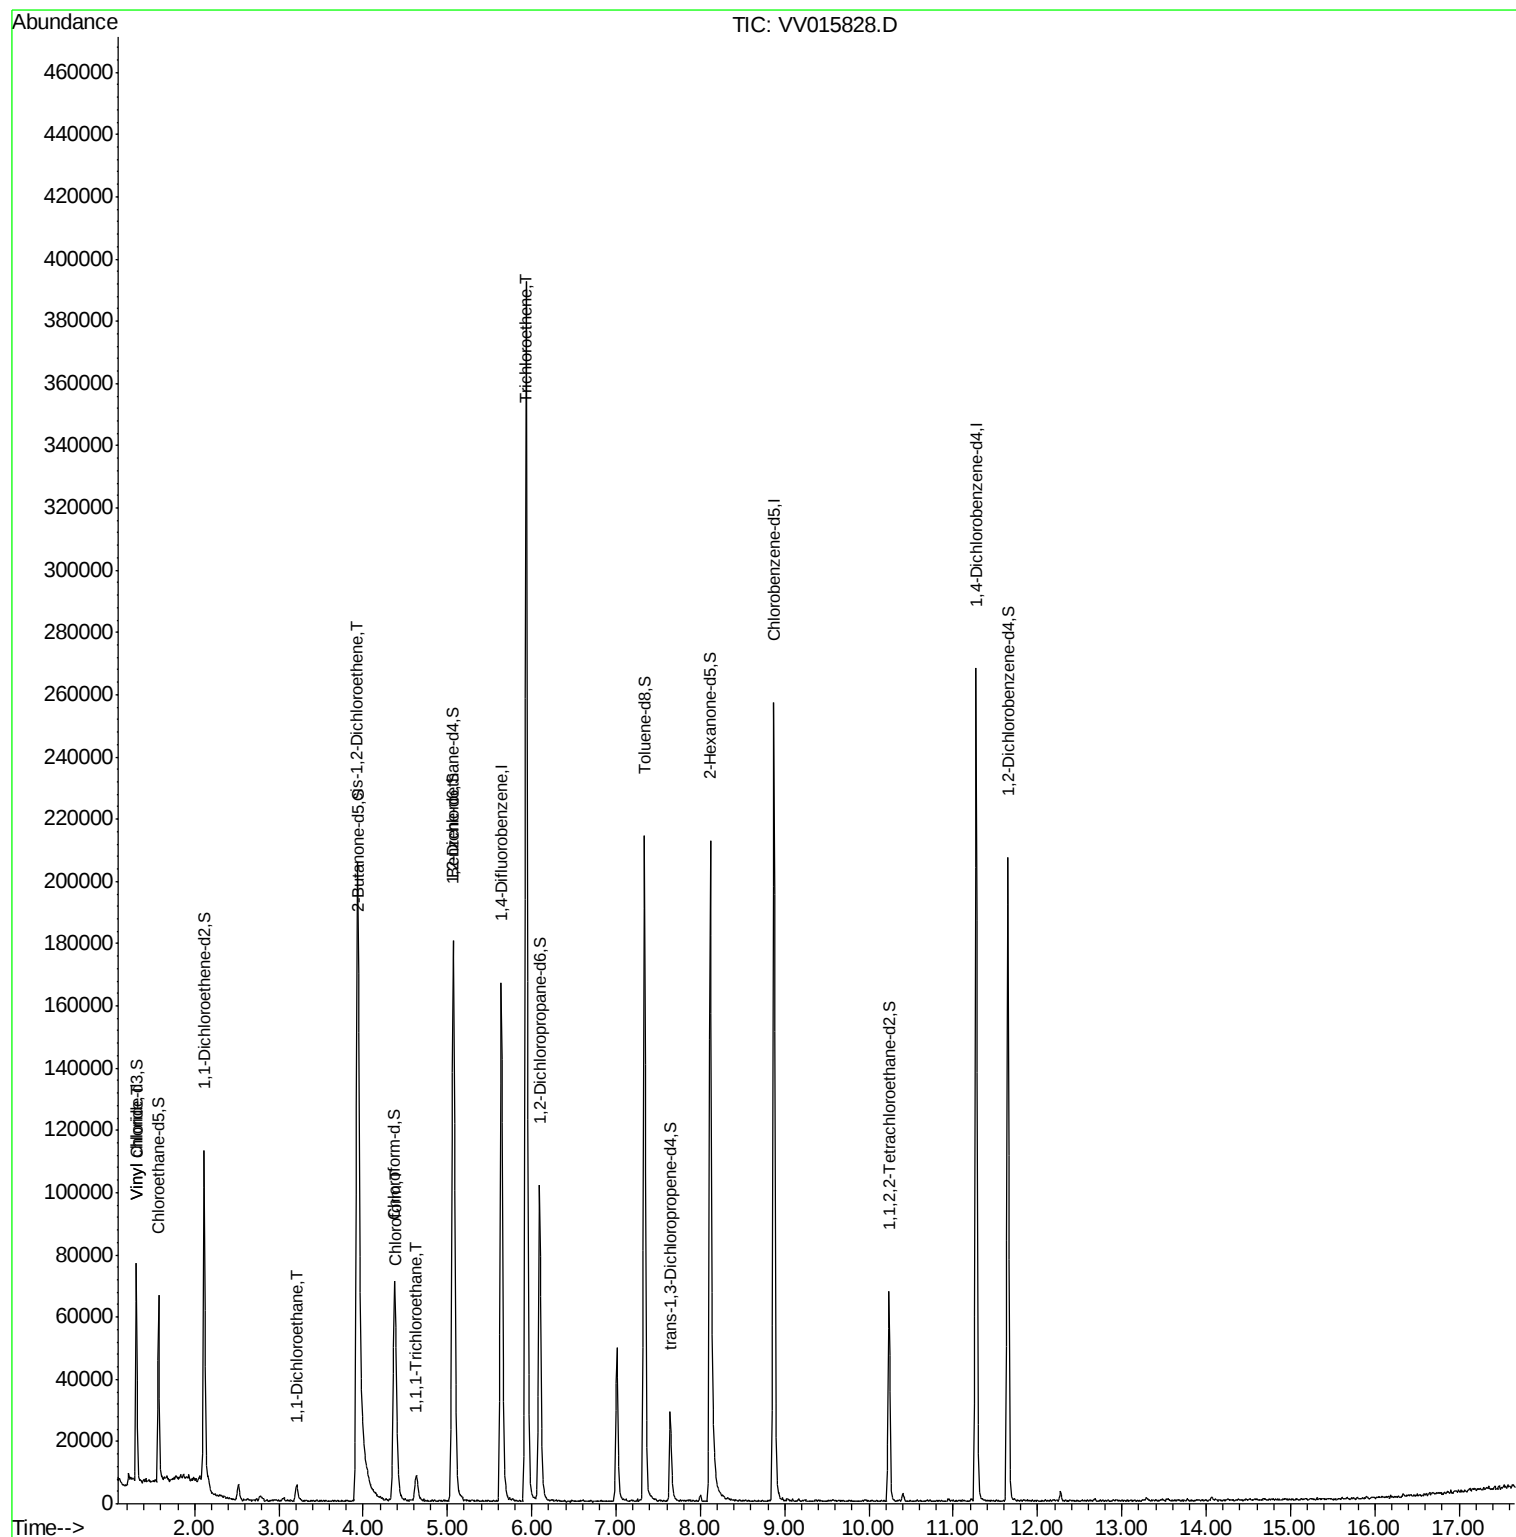

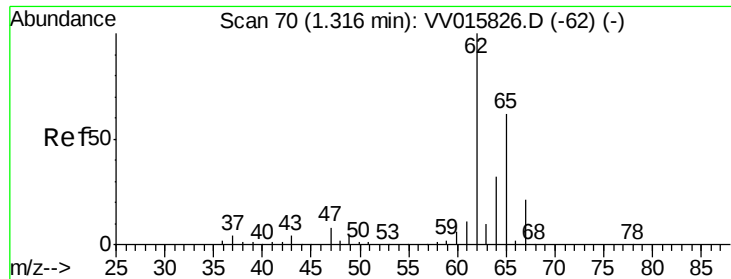

#5

Vinyl chloride

Concen: 0.350 ug/L

RT: 1.32 min Scan# 70

Delta R.T. 0.00 min

Lab File: VV015828.D

Acq: 30 Apr 2020 11:48

Instrument :

MSVOA_V

ClientSampled :





BFSB0DL

Tot Ion: 62 Resp: 3710

Ion Ratio Lower Upper

62 100

64 50.2 22.7 42.1#

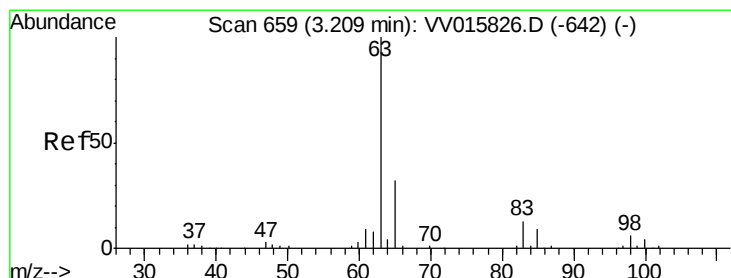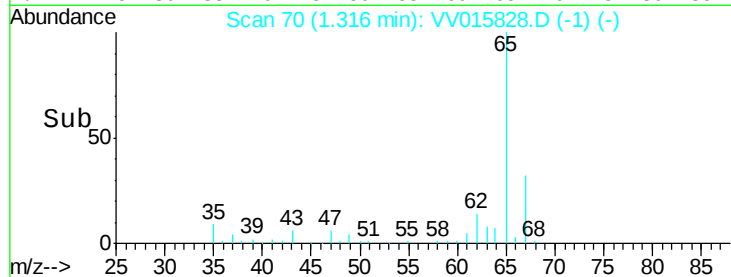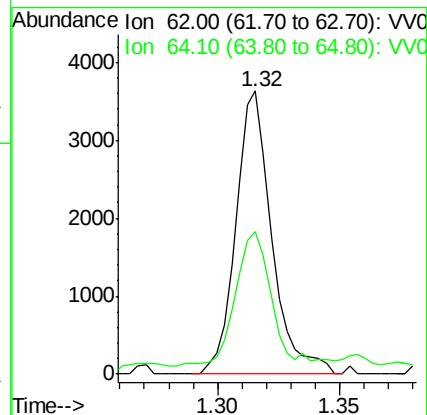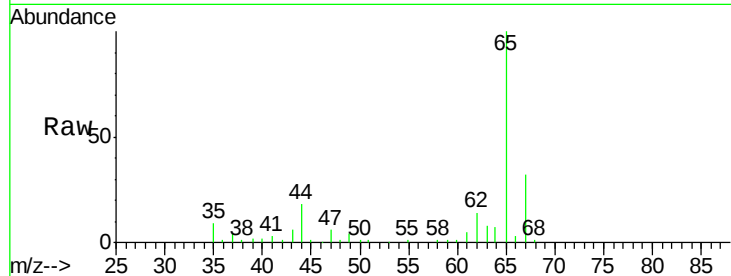

#19

1,1-Dichloroethane

Concen: 0.304 ug/L

RT: 3.21 min Scan# 659

Delta R.T. 0.00 min

Lab File: VV015828.D

Acq: 30 Apr 2020 11:48




Tgt Ion: 63 Resp: 5221


Ion Ratio Lower Upper

63 100

65 35.3 22.3 41.3

83 13.3 9.3 17.3


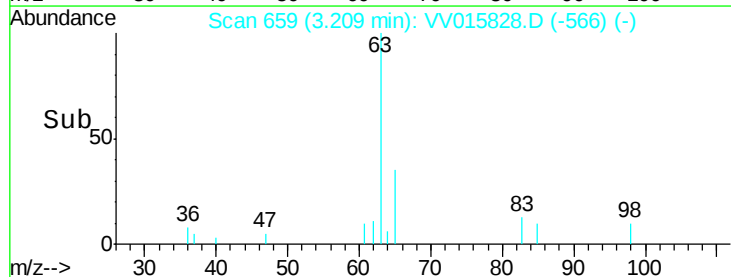
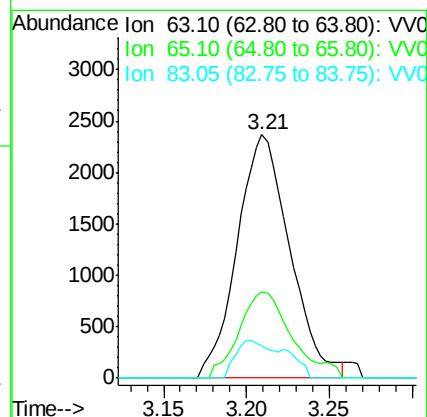
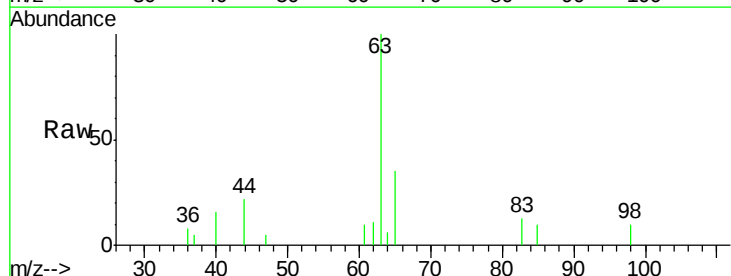


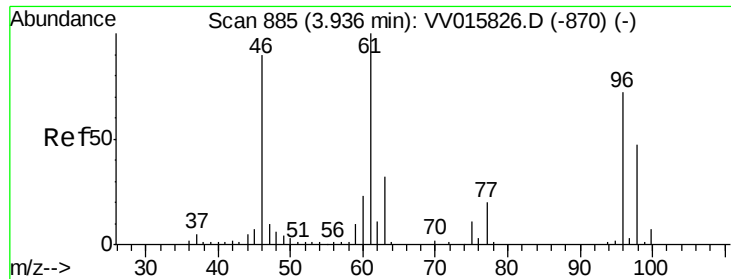

#22
 cis-1,2-Dichloroethene
 Concen: 10.360 ug/L
 RT: 3.93 min Scan# 884
 Delta R.T. -0.00 min
 Lab File: VV015828.D
 Acq: 30 Apr 2020 11:48




Instrument :
 MSVOA_V
 ClientSampleId :
 BFSB0DL


Tot Ion: 96 Resp: 100119
 Ion Ratio Lower Upper
 96 100
 61 144.1 96.4 179.0
 68 0.0 0.0 0.0

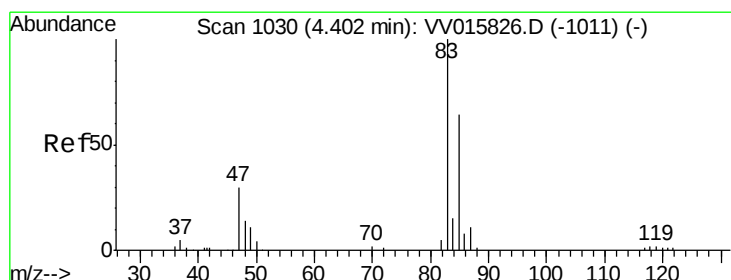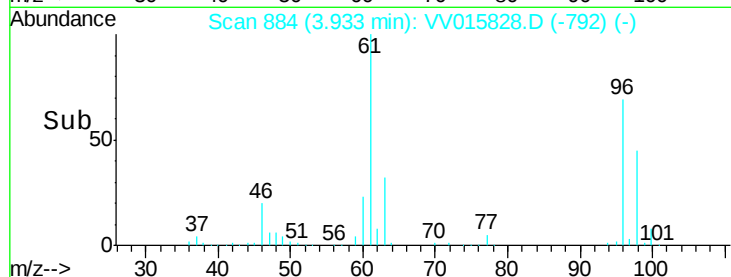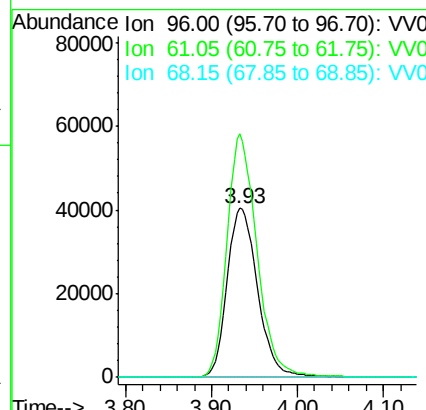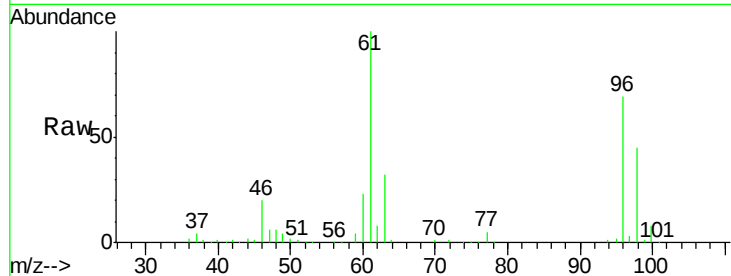

#25
 Chloroform
 Concen: 0.484 ug/L
 RT: 4.40 min Scan# 1028
 Delta R.T. -0.01 min
 Lab File: VV015828.D
 Acq: 30 Apr 2020 11:48

Tgt Ion: 83 Resp: 8817
 Ion Ratio Lower Upper
 83 100
 85 66.0 46.1 85.5


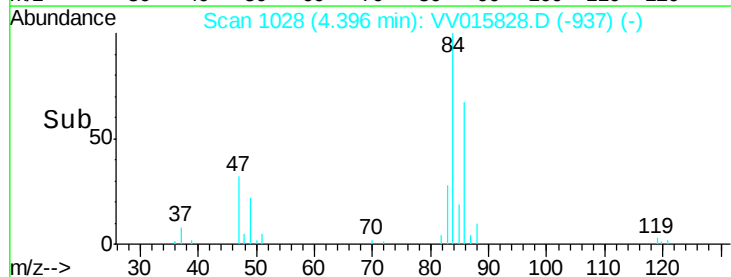
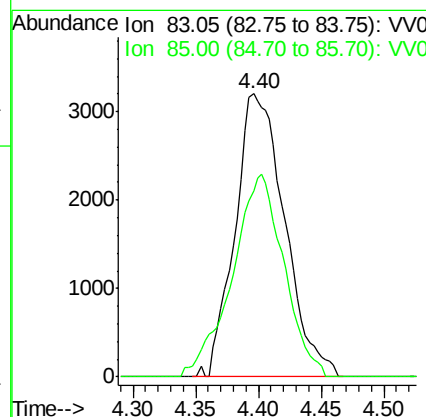
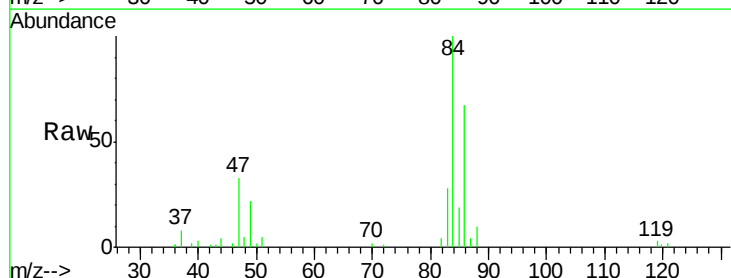


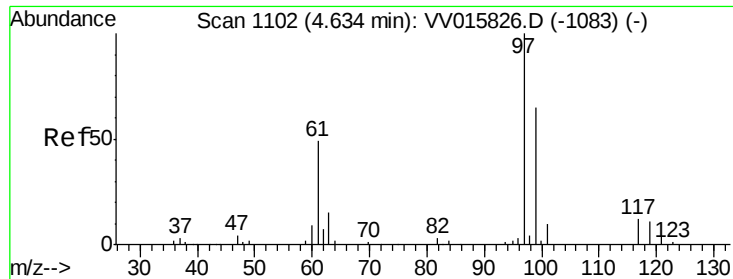

#29
 1,1,1-Trichloroethane
 Concen: 0.441 ug/L
 RT: 4.63 min Scan# 1101
 Delta R.T. -0.00 min
 Lab File: VV015828.D
 Acq: 30 Apr 2020 11:48

Instrument :
 MSVOA_V
 ClientSampleId :
 BFSB0DL

Tot Ion: 97 Resp: 7160
 Ion Ratio Lower Upper
 97 100
 99 62.0 51.6 77.4
 61 49.3 38.6 57.8

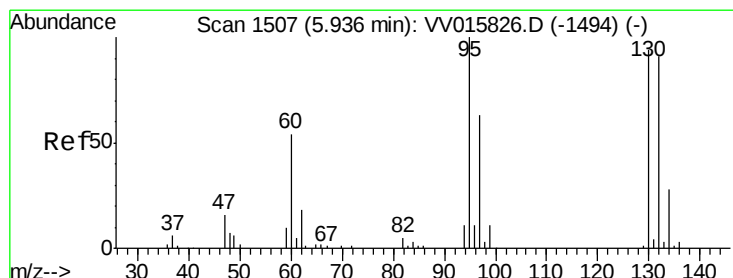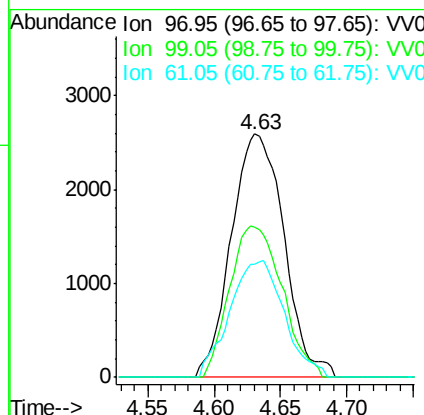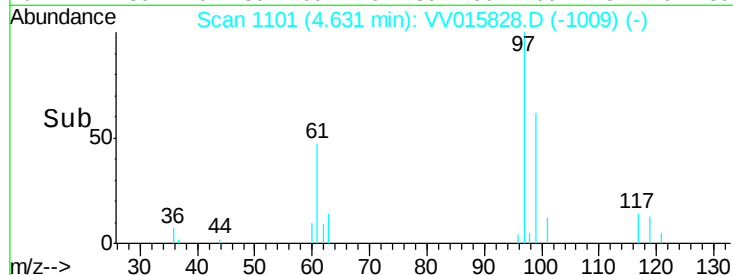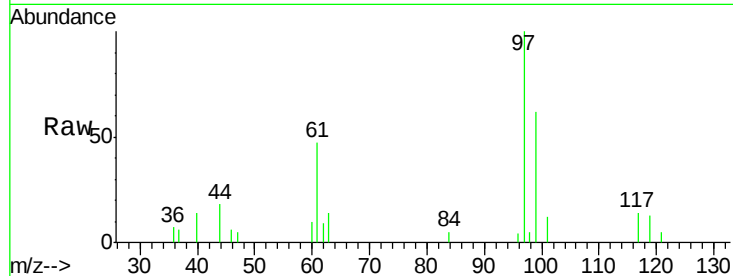

#34
 Trichloroethene
 Concen: 13.514 ug/L
 RT: 5.94 min Scan# 1507
 Delta R.T. 0.00 min
 Lab File: VV015828.D
 Acq: 30 Apr 2020 11:48

Tgt Ion: 95 Resp: 136574
 Ion Ratio Lower Upper
 95 100
 97 65.8 44.7 82.9
 132 91.8 65.2 121.0
 130 95.4 65.0 120.6

