

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV043020\
 Data File : VV015839.D
 Acq On : 30 Apr 2020 17:23
 Operator : SY/MD
 Sample : L2413-22
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: May 01 03:19:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri May 01 01:42:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	123322	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.87	117	119617	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.27	152	55248	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	36021	5.59	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	111.80%
7) Chloroethane-d5	1.57	69	32859	5.29	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.80%
11) 1,1-Dichloroethene-d2	2.12	63	53346	3.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.60%
20) 2-Butanone-d5	3.97	46	96513	46.64	ug/L	0.05
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.28%
24) Chloroform-d	4.38	84	67168	4.47	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.40%
26) 1,2-Dichloroethane-d4	5.06	65	42031	5.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.00%
32) Benzene-d6	5.07	84	139114	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.40%
36) 1,2-Dichloropropane-d6	6.10	67	43093	4.72	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.40%
41) Toluene-d8	7.34	98	122309	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.20%
43) trans-1,3-Dichloropropene-	7.65	79	14961	4.24	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.80%
46) 2-Hexanone-d5	8.12	63	67462	39.21	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	78.42%
57) 1,1,2,2-Tetrachloroethane-	10.24	84	29253	4.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.20%
64) 1,2-Dichlorobenzene-d4	11.65	152	44546	4.74	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.80%


Target Compounds					Ovalue
25) Chloroform	4.41	83	6426	0.384 ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV043020\
Data File : VV015839.D
Acq On : 30 Apr 2020 17:23
Operator : SY/MD
Sample : L2413-22
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: May 01 03:19:28 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri May 01 01:42:43 2020
Response via : Initial Calibration

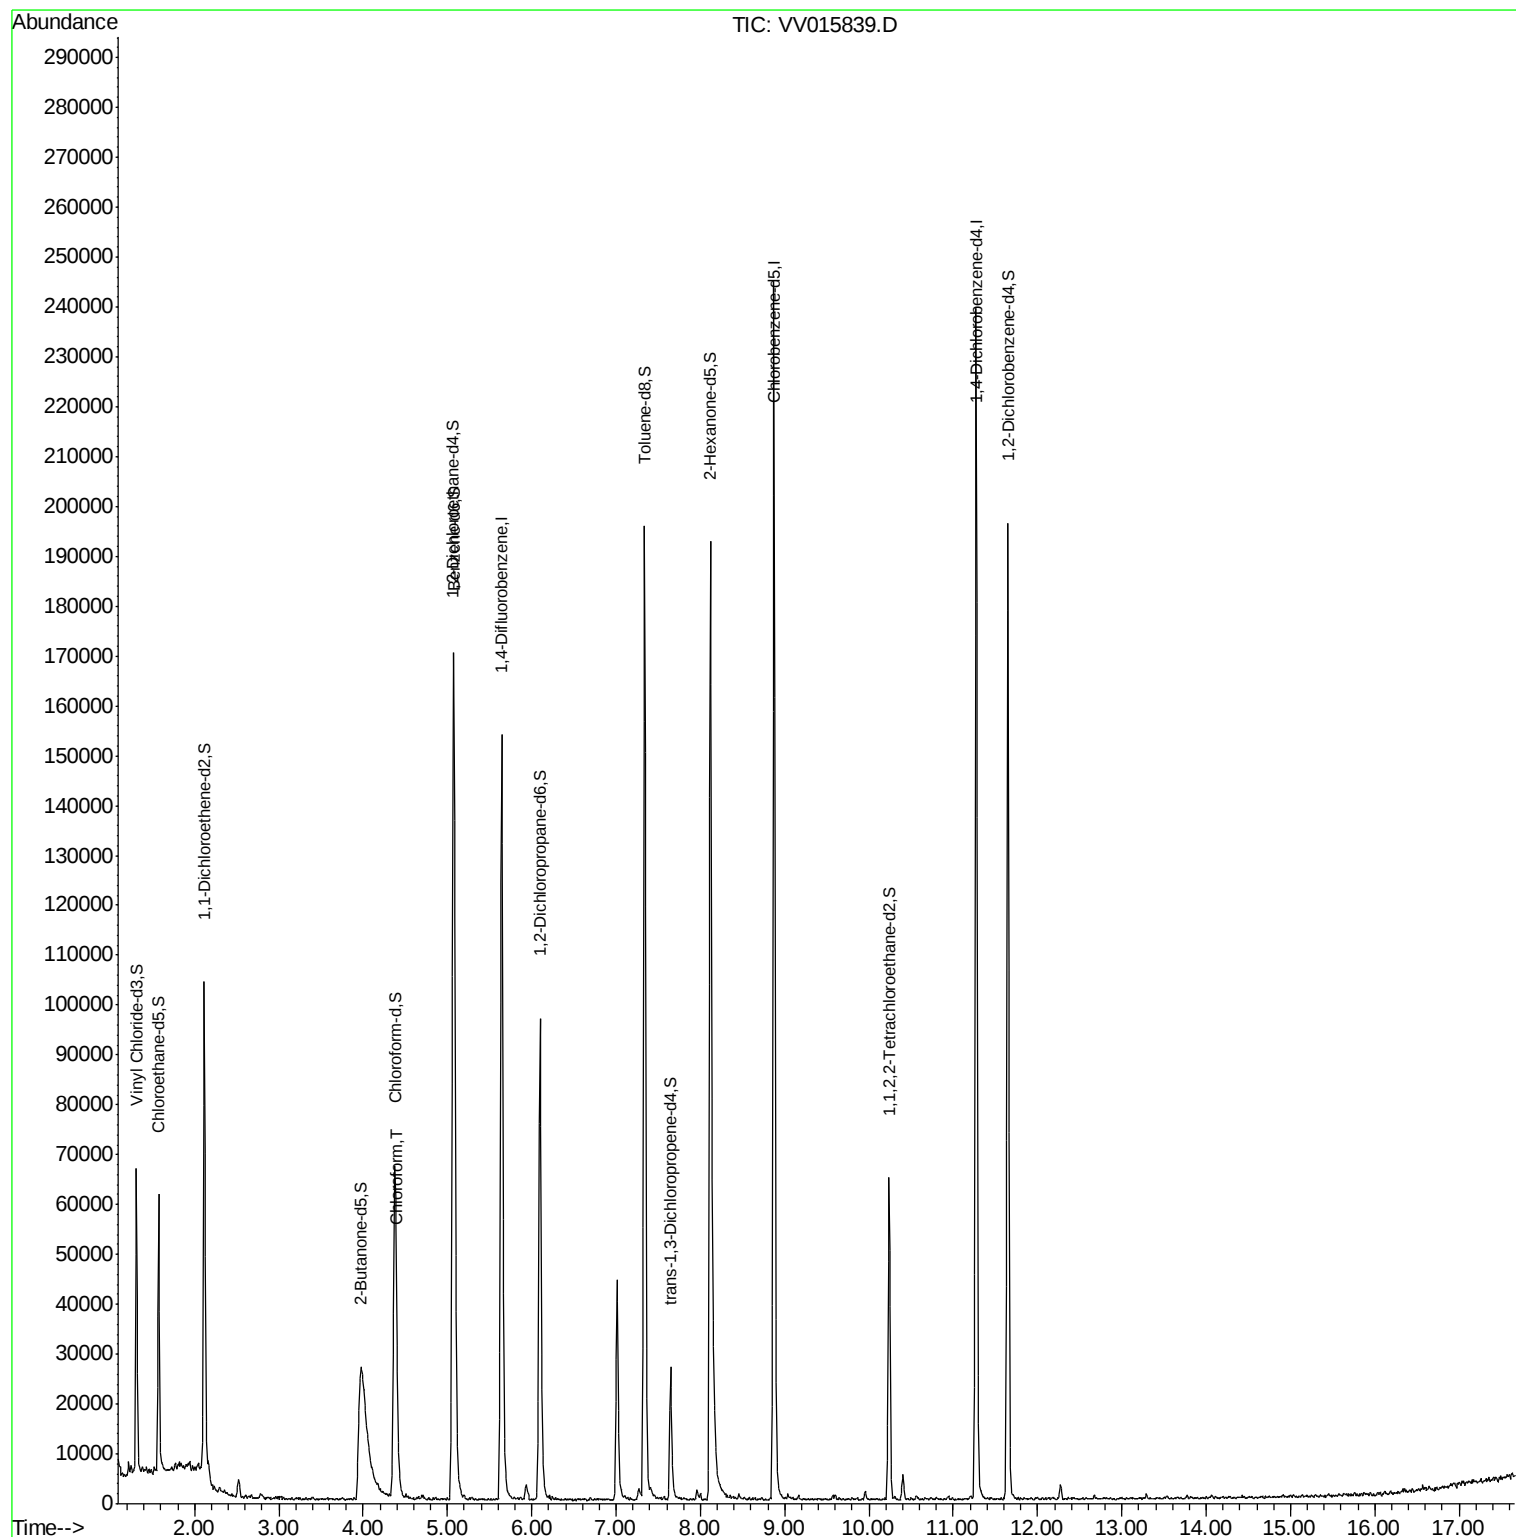

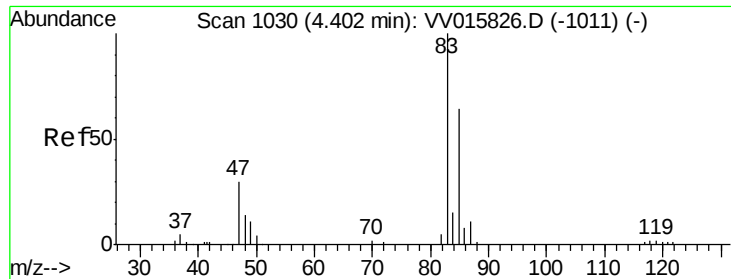

#25
 Chloroform
 Concen: 0.384 ug/L
 RT: 4.41 min Scan# 1031
 Delta R.T. 0.00 min
 Lab File: VV015839.D
 Acq: 30 Apr 2020 17:23

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Tot Ion: 83 Resp: 6426
 Ion Ratio Lower Upper
 83 100
 85 79.1 46.1 85.5

