

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV043020\
 Data File : VV015828.D
 Acq On : 30 Apr 2020 11:48
 Operator : SY/MD
 Sample : L2421-09DL 100X
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFSB0DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	81	rVB	70186	75358	9.70%	1.457%
2	1.573	143	150	160	rBV	59894	68597	8.83%	1.326%
3	2.116	309	319	330	rBV	105364	153524	19.76%	2.967%
4	2.521	432	445	456	rBV3	4876	8742	1.13%	0.169%
5	3.213	647	660	670	rBV3	5235	11083	1.43%	0.214%
6	3.933	868	884	939	rBV2	205270	627764	80.80%	12.134%
7	4.373	1005	1021	1044	rBV2	70241	192064	24.72%	3.712%
8	4.631	1087	1101	1102	rBV2	8126	12420	1.60%	0.240%
9	5.071	1222	1238	1258	rBV2	180254	442026	56.89%	8.544%
10	5.640	1402	1415	1443	rBV	166625	342140	44.04%	6.613%
11	5.936	1492	1507	1535	rBV	392097	776971	100.00%	15.017%
12	6.093	1542	1556	1584	rVB2	101061	216317	27.84%	4.181%
13	7.010	1826	1841	1863	rBV	49273	93162	11.99%	1.801%
14	7.338	1929	1943	1967	rBV	213418	376135	48.41%	7.270%
15	7.643	2028	2038	2057	rBV2	28760	52910	6.81%	1.023%
16	8.116	2173	2185	2222	rBV	212247	443954	57.14%	8.581%
17	8.872	2409	2420	2437	rBV	256479	423722	54.54%	8.190%
18	10.238	2834	2845	2861	rBV	67374	108346	13.94%	2.094%
19	11.270	3155	3166	3185	rBV	267748	417547	53.74%	8.070%
20	11.646	3272	3283	3304	rBV	206677	331000	42.60%	6.398%


Sum of corrected areas: 5173782

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV043020\
Data File : VV015828.D
Acq On : 30 Apr 2020 11:48
Operator : SY/MD
Sample : L2421-09DL 100X
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFSB0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

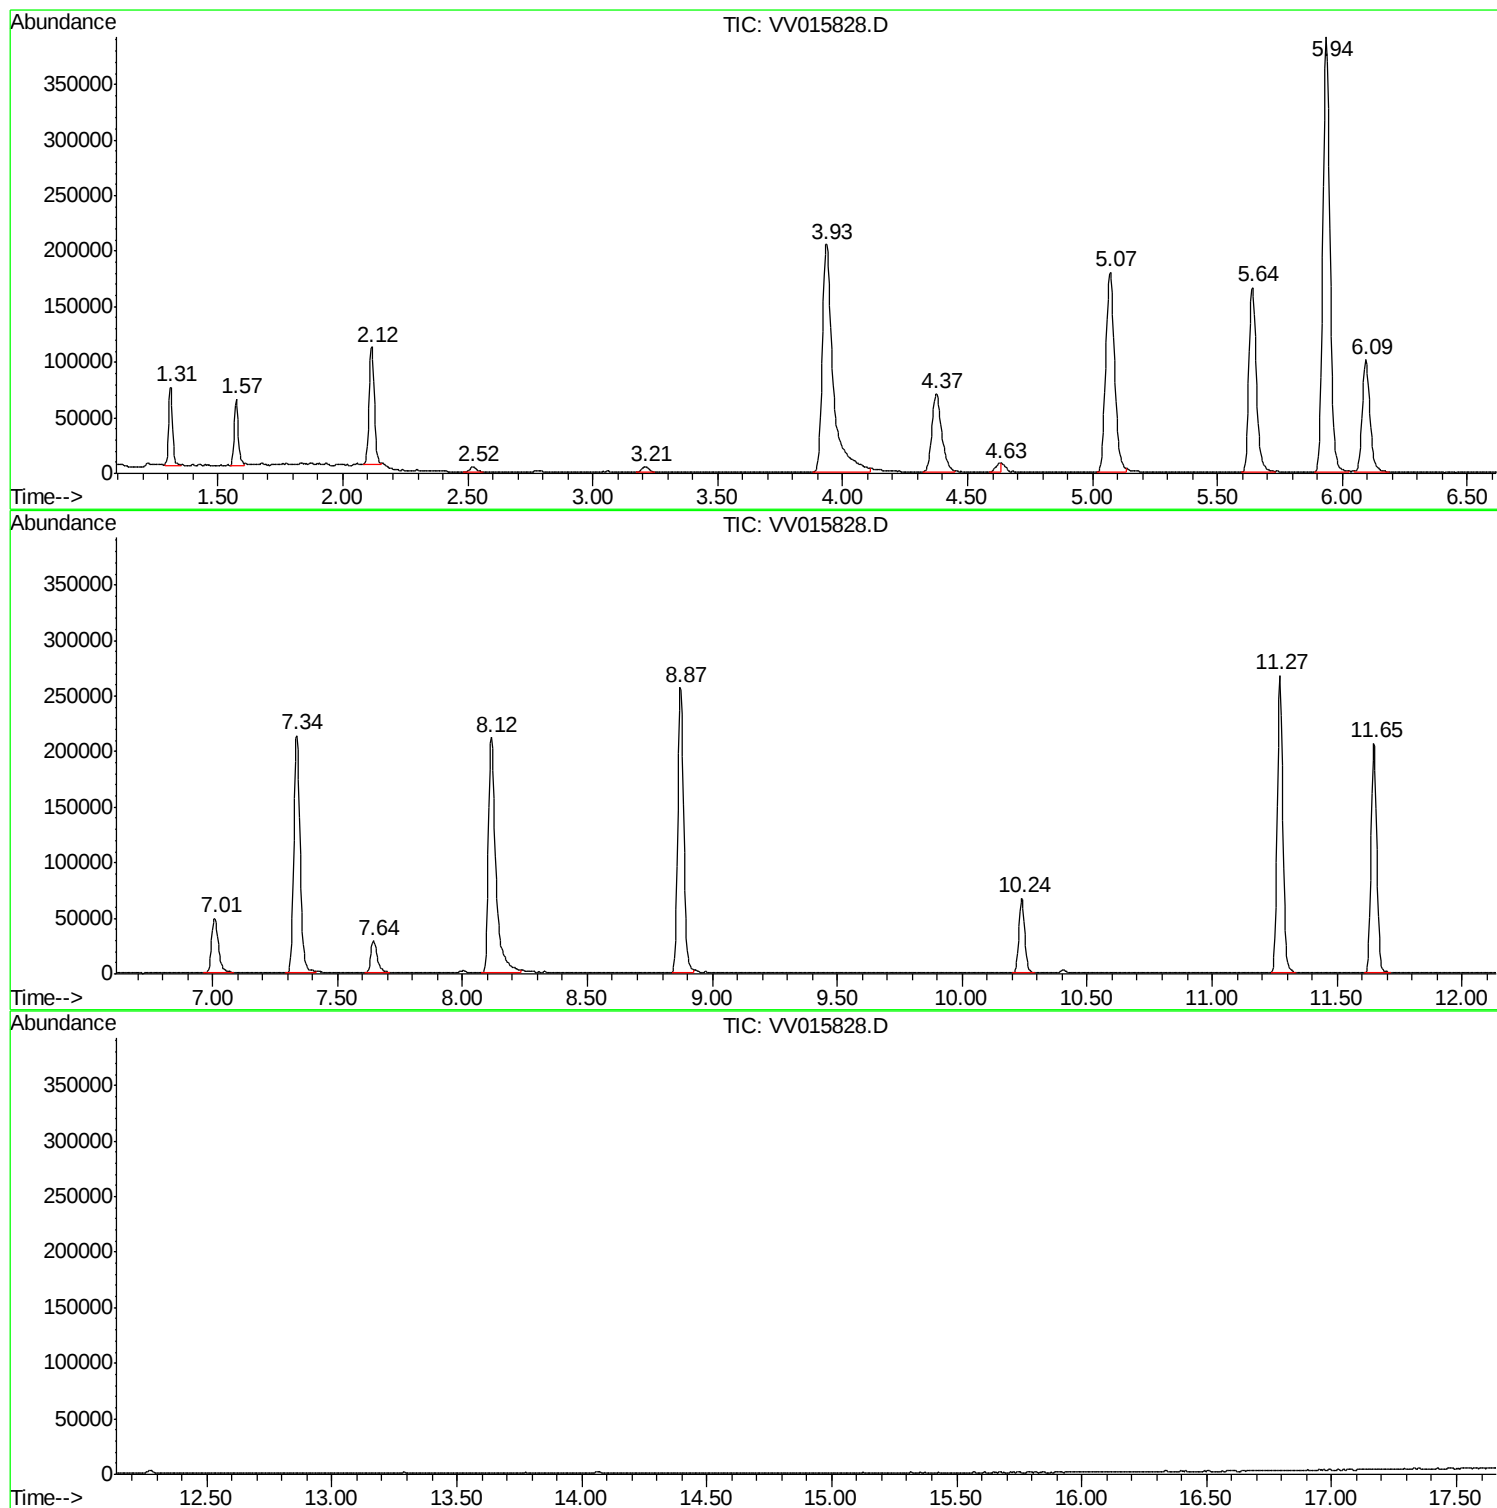

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV043020\
Data File : VV015828.D
Acq On : 30 Apr 2020 11:48
Operator : SY/MD
Sample : L2421-09DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFSB0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV043020\
Data File : VV015828.D
Acq On : 30 Apr 2020 11:48
Operator : SY/MD
Sample : L2421-09DL 100X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFSB0DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc