


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV043020\
 Data File : VV015825.D
 Acq On : 30 Apr 2020 09:27
 Operator : SY/MD
 Sample : BFB47
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB47

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri May 01 11:41:06 2020

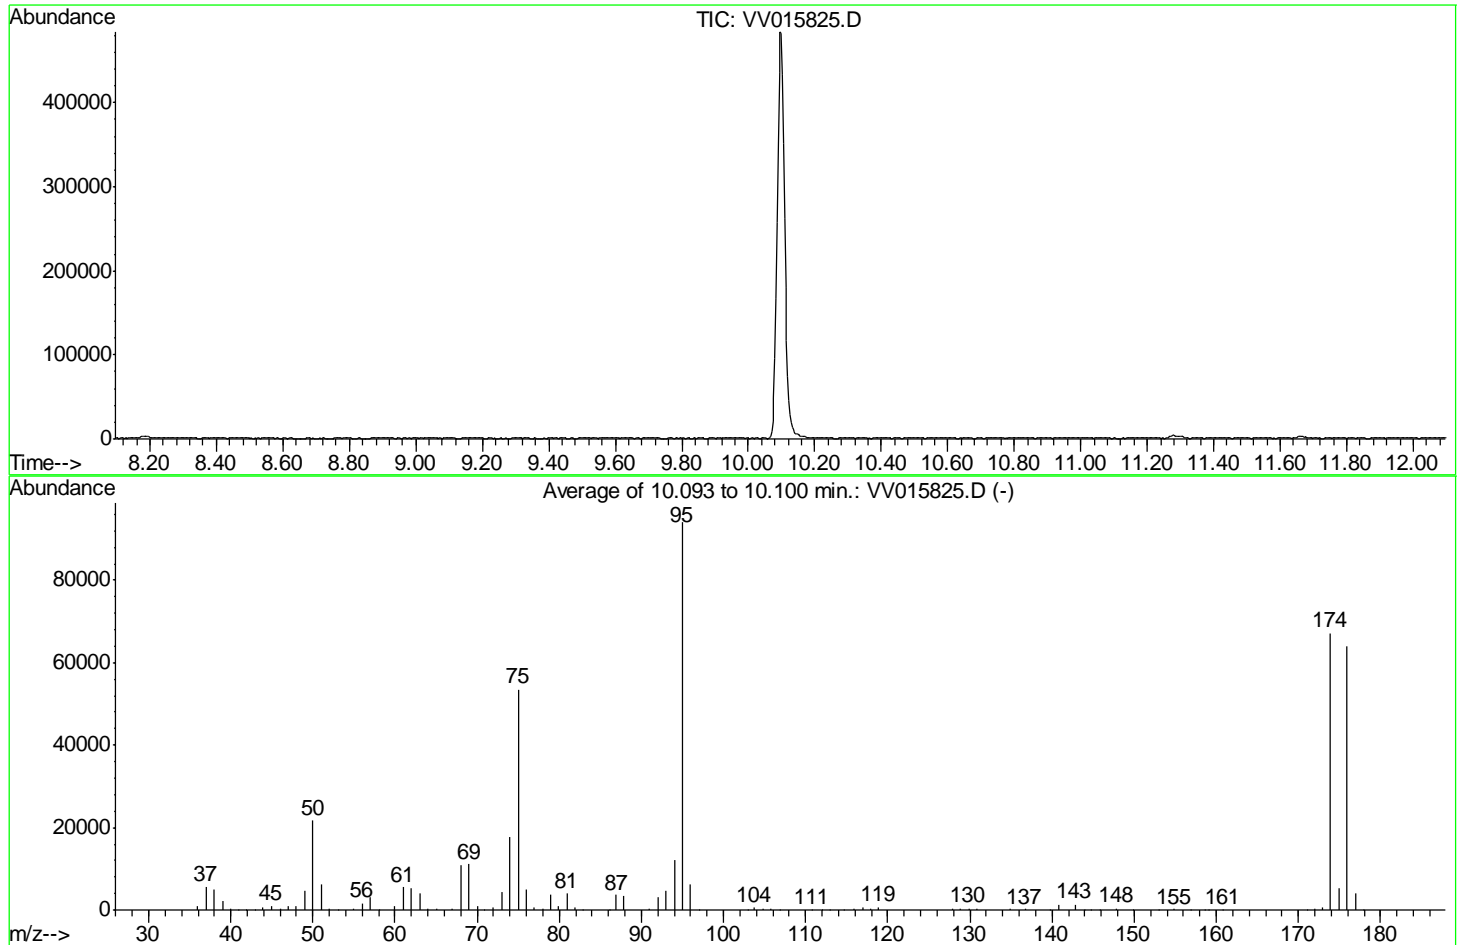

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	21648	PASS
75	95	30	80	57.0	53562	PASS
95	95	100	100	100.0	94048	PASS
96	95	5	9	6.6	6239	PASS
173	174	0.00	2	0.9	607	PASS
174	95	50	120	71.3	67090	PASS
175	174	5	9	7.8	5241	PASS
176	174	95	101	95.4	63997	PASS
177	176	5	9	6.4	4072	PASS

m/z	Abundance
36.00	950.0
37.00	5556.0
38.00	4696.0
39.00	1971.0
40.00	467.0
43.00	104.0
43.90	1213.0
44.90	1030.0
46.00	192.0
47.00	1027.0
47.90	793.0
49.00	4337.0
50.00	20336.0
51.00	5913.0
52.00	295.0
53.00	115.0
54.90	379.0
56.00	1613.0
57.00	2939.0
58.20	109.0
60.00	952.0
61.00	5215.0
62.00	4923.0
63.00	4091.0
64.00	434.0
65.00	320.0
66.90	330.0
68.00	10230.0
69.00	10741.0
70.00	882.0
72.00	481.0
73.00	4416.0
74.00	16744.0
75.00	50016.0
76.00	4565.0
77.00	475.0
77.90	364.0
78.90	3487.0
80.00	1024.0
80.90	3553.0
81.90	700.0
82.90	118.0
86.10	133.0
87.00	3418.0
87.90	3030.0
90.90	421.0
92.00	2928.0
93.00	4266.0
94.00	11527.0
95.00	88480.0
96.00	5989.0
96.90	175.0
103.80	581.0
104.80	245.0
105.80	422.0
106.90	116.0
110.80	144.0
112.00	102.0
112.80	134.0
115.90	374.0
116.90	586.0
117.80	376.0
118.80	604.0
127.90	412.0
128.90	202.0
129.90	369.0
130.80	179.0
134.80	170.0
136.80	216.0
139.70	122.0
140.80	1193.0
142.80	1144.0
144.70	153.0
145.80	114.0
147.80	286.0
149.80	146.0
154.90	197.0
156.90	148.0
158.70	104.0
160.80	113.0
172.00	367.0
173.00	844.0
173.90	60576.0
175.00	4822.0
175.90	58080.0
177.00	3727.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
36.00	1056.0
37.00	5928.0
38.00	5068.0
39.00	2124.0
40.00	556.0
40.90	114.0
41.90	110.0
43.00	112.0
43.90	1197.0
44.90	1066.0
46.00	204.0
47.00	1132.0
47.90	878.0
49.00	4639.0
50.00	22552.0
51.00	6475.0
52.00	315.0
53.00	110.0
54.90	443.0
56.00	1614.0
57.00	3165.0
58.00	150.0
60.00	972.0
61.00	5706.0
62.00	5436.0
63.00	4170.0
64.00	443.0
65.00	344.0
66.90	371.0
68.00	11392.0
69.00	11525.0
70.00	979.0
72.00	537.0
73.00	4615.0
74.00	18232.0
75.00	55480.0
76.00	5083.0
76.90	500.0
78.00	389.0
78.90	3872.0
80.00	1114.0
80.90	4084.0
81.90	739.0
82.90	152.0
86.00	111.0
87.00	3832.0
87.90	3458.0
90.90	466.0
92.00	3263.0
93.00	4814.0
94.00	12634.0
95.00	97512.0
96.00	6447.0
97.00	140.0
103.80	544.0
104.80	263.0
105.80	421.0
106.90	138.0
110.80	143.0
112.80	120.0
115.90	383.0
116.90	639.0
117.90	417.0
118.90	676.0
127.90	449.0
128.90	225.0
129.90	458.0
130.90	183.0
134.90	198.0
136.80	219.0
139.70	130.0
140.90	1264.0
142.80	1297.0
144.00	105.0
144.70	167.0
145.70	130.0
147.90	343.0
149.80	147.0
153.00	102.0
154.90	219.0
156.80	160.0
158.60	119.0
171.10	111.0
171.90	420.0
173.00	979.0
173.90	69480.0
175.00	5459.0
175.90	65904.0
176.90	4209.0
177.90	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
35.90	1088.0
37.00	5730.0
38.00	5003.0
39.00	2135.0
40.00	594.0
40.90	105.0
41.90	140.0
43.00	123.0
44.00	1090.0
44.90	969.0
46.10	183.0
46.90	1124.0
47.90	859.0
49.00	4631.0
50.00	22056.0
51.00	6440.0
52.00	290.0
54.90	425.0
56.00	1561.0
57.00	3197.0
58.00	217.0
60.00	940.0
61.00	5535.0
62.00	5365.0
63.00	3978.0
64.00	414.0
65.00	379.0
66.90	328.0
68.00	11263.0
69.00	11198.0
70.00	943.0
70.90	102.0
72.00	492.0
73.00	4390.0
74.00	18352.0
75.00	55192.0
76.00	4969.0
76.90	512.0
78.00	386.0
78.90	3975.0
79.90	1073.0
80.90	4154.0
81.90	771.0
82.90	174.0
86.00	102.0
86.90	3776.0
87.90	3665.0
90.90	447.0
92.00	3267.0
93.00	4723.0
94.00	12416.0
95.00	96152.0
96.00	6283.0
97.10	138.0
102.90	107.0
103.80	474.0
104.90	255.0
105.80	374.0
106.90	135.0
110.70	136.0
112.90	108.0
114.70	107.0
115.90	384.0
116.90	650.0
117.90	413.0
118.90	664.0
127.90	405.0
128.80	222.0
129.90	445.0
130.90	157.0
134.90	196.0
136.70	201.0
139.80	121.0
140.90	1199.0
142.90	1295.0
144.70	175.0
145.70	130.0
147.80	375.0
149.80	113.0
153.00	114.0
154.90	228.0
157.00	167.0
158.60	111.0
159.00	111.0
171.90	435.0
173.90	71216.0
175.00	5443.0
175.90	68008.0
176.90	4280.0
177.90	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

Scan 2788 (10.055 min): VV015825.D
BFB47

m/z	Abundance
39.90	345.0
43.90	435.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47