


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050119\
Data File : VV010599.D
Acq On : 01 May 2019 09:25
Operator : SY/MD
Sample : BFB41
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB41

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR050119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu May 02 08:18:34 2019

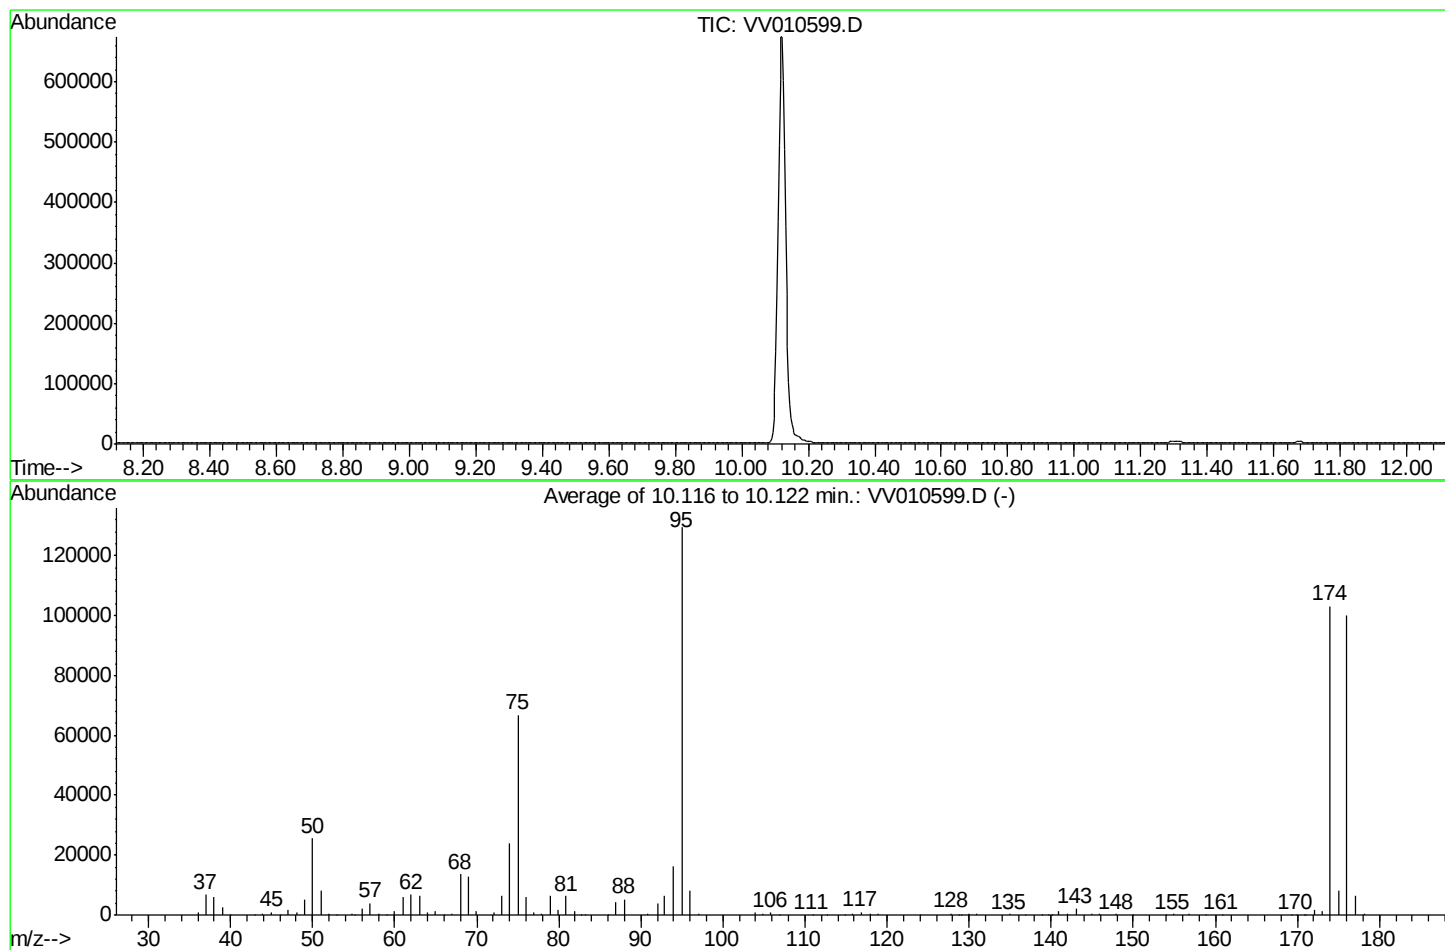

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	25645	PASS
75	95	30	80	51.7	66896	PASS
95	95	100	100	100.0	129474	PASS
96	95	5	9	6.2	8092	PASS
173	174	0.00	2	1.4	1494	PASS
174	95	50	120	79.7	103202	PASS
175	174	5	9	7.9	8150	PASS
176	174	95	101	96.9	99954	PASS
177	176	5	9	6.6	6612	PASS

Scan 2794 (10.074 min): VV010599.D
BFB41

m/z	Abundance
39.90	1422.0
40.80	105.0
43.90	389.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
36.10	1027.0
37.00	6173.0
38.00	5617.0
39.00	2320.0
39.90	1353.0
43.00	119.0
43.90	793.0
45.00	863.0
46.90	1322.0
48.10	922.0
49.00	5148.0
50.00	23968.0
51.00	7692.0
52.00	512.0
52.90	121.0
54.90	250.0
55.10	249.0
56.00	2236.0
57.00	3522.0
57.90	264.0
60.00	1283.0
61.00	5353.0
62.00	6320.0
63.00	6077.0
63.90	785.0
65.00	993.0
66.10	157.0
67.00	303.0
68.00	13108.0
69.00	11803.0
69.90	1165.0
72.00	745.0
73.00	6183.0
74.00	21808.0
75.00	63208.0
76.00	5860.0
76.90	751.0
78.00	499.0
78.90	6412.0
80.00	1389.0
80.90	5997.0
82.00	1182.0
82.80	145.0
86.10	166.0
86.90	4018.0
88.00	5011.0
90.90	501.0
92.00	3750.0
92.90	5955.0
94.00	14776.0
95.00	122056.0
96.00	7680.0
97.00	302.0
103.90	583.0
104.90	257.0
105.80	726.0
106.90	207.0
112.70	117.0
114.80	145.0
115.80	395.0
116.80	938.0
117.90	596.0
118.90	706.0
124.10	119.0
127.90	512.0
128.80	329.0
130.00	386.0
130.90	271.0
135.00	356.0
137.10	149.0
138.80	100.0
140.10	193.0
141.00	1499.0
142.10	291.0
143.00	1714.0
144.90	382.0
146.00	275.0
147.90	364.0
154.90	220.0
156.70	173.0
158.80	124.0
160.90	136.0
169.30	106.0
169.90	133.0
172.00	1569.0
173.00	1456.0
174.00	93280.0
175.00	7787.0
176.00	90888.0
177.00	6161.0
178.10	249.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
36.10	1145.0
37.00	7006.0
38.00	6036.0
39.00	2661.0
39.90	1502.0
43.00	152.0
43.90	1002.0
45.00	897.0
46.10	162.0
47.00	1726.0
48.10	1023.0
49.00	5405.0
50.00	26656.0
51.00	8432.0
52.00	461.0
52.90	167.0
54.80	289.0
56.00	2302.0
57.00	4056.0
58.00	250.0
60.00	1260.0
61.00	6170.0
62.00	7061.0
63.00	6449.0
64.00	798.0
65.00	1275.0
66.00	145.0
67.00	381.0
68.00	14190.0
69.00	13407.0
69.90	1202.0
72.10	824.0
73.00	6815.0
74.00	24664.0
75.00	68992.0
76.00	6369.0
76.90	730.0
78.00	412.0
78.90	6891.0
79.90	1579.0
80.90	6556.0
82.00	1305.0
82.70	103.0
83.20	154.0
86.10	217.0
86.90	4520.0
87.90	5469.0
90.80	611.0
92.00	4169.0
92.90	6834.0
94.00	16712.0
95.00	134208.0
96.00	8330.0
97.00	428.0
103.90	694.0
104.80	325.0
105.80	803.0
106.80	191.0
110.90	163.0
112.70	141.0
114.80	165.0
115.80	418.0
116.80	1068.0
117.90	535.0
118.90	644.0
124.10	126.0
127.80	689.0
129.00	344.0
129.90	452.0
130.90	269.0
134.90	405.0
136.90	183.0
138.80	125.0
140.00	224.0
140.90	1544.0
142.00	318.0
143.00	1979.0
144.90	481.0
145.90	247.0
148.00	335.0
154.00	113.0
154.90	288.0
156.80	290.0
158.70	160.0
160.90	245.0
169.90	129.0
170.80	232.0
172.10	1689.0
173.00	1518.0
174.00	106864.0
175.00	8371.0
176.00	103448.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

177.006859.0

178.20257.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

m/z	Abundance
36.10	1000.0
37.00	7087.0
38.00	5737.0
39.00	2617.0
39.90	1487.0
43.00	194.0
43.90	1085.0
45.00	864.0
46.00	214.0
46.90	1622.0
48.00	1004.0
49.00	5223.0
50.00	26312.0
51.00	8063.0
52.10	389.0
52.90	197.0
54.80	346.0
56.00	2103.0
57.00	4052.0
58.10	202.0
59.00	105.0
60.00	1124.0
61.00	6564.0
62.00	7055.0
63.00	6162.0
64.00	757.0
65.00	1350.0
66.00	132.0
67.00	410.0
68.00	13496.0
69.00	13867.0
69.90	1194.0
72.10	767.0
73.00	6465.0
74.00	25360.0
75.00	68488.0
76.00	5954.0
77.00	695.0
77.80	338.0
78.90	6311.0
79.90	1624.0
80.90	6225.0
81.90	1320.0
83.10	154.0
85.90	204.0
87.00	4808.0
87.90	5372.0
90.80	643.0
92.00	4233.0
92.90	6806.0
94.00	16864.0
95.00	132160.0
96.00	8268.0
97.00	370.0
103.80	750.0
104.80	342.0
105.80	791.0
106.80	211.0
110.90	198.0
112.70	132.0
114.80	159.0
115.80	360.0
116.80	1041.0
117.90	473.0
118.90	557.0
127.80	745.0
128.70	264.0
129.10	303.0
129.90	520.0
130.90	295.0
134.90	359.0
136.80	253.0
138.80	111.0
139.60	129.0
140.10	159.0
140.90	1483.0
142.00	255.0
143.00	2170.0
144.90	540.0
145.80	237.0
148.00	320.0
149.90	126.0
154.80	349.0
156.90	354.0
158.70	180.0
160.80	284.0
169.80	101.0
171.00	327.0
172.10	1896.0
173.00	1509.0
174.00	109464.0
175.00	8293.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41

176.00	105528.0
177.00	6817.0
178.20	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB41