
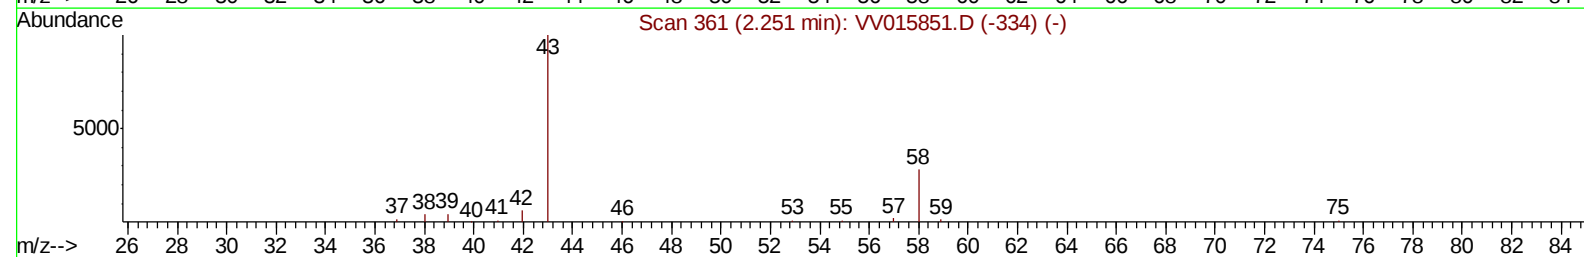
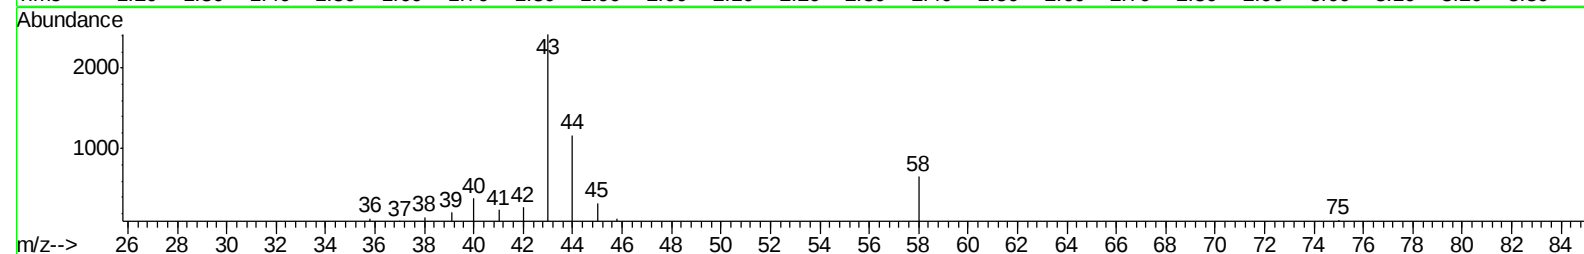


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050120\
 Data File : VV015853.D
 Acq On : 01 May 2020 12:37
 Operator : SY/MD
 Sample : L2416-11
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: May 02 00:25:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat May 02 00:06:27 2020
 Response via : Initial Calibration

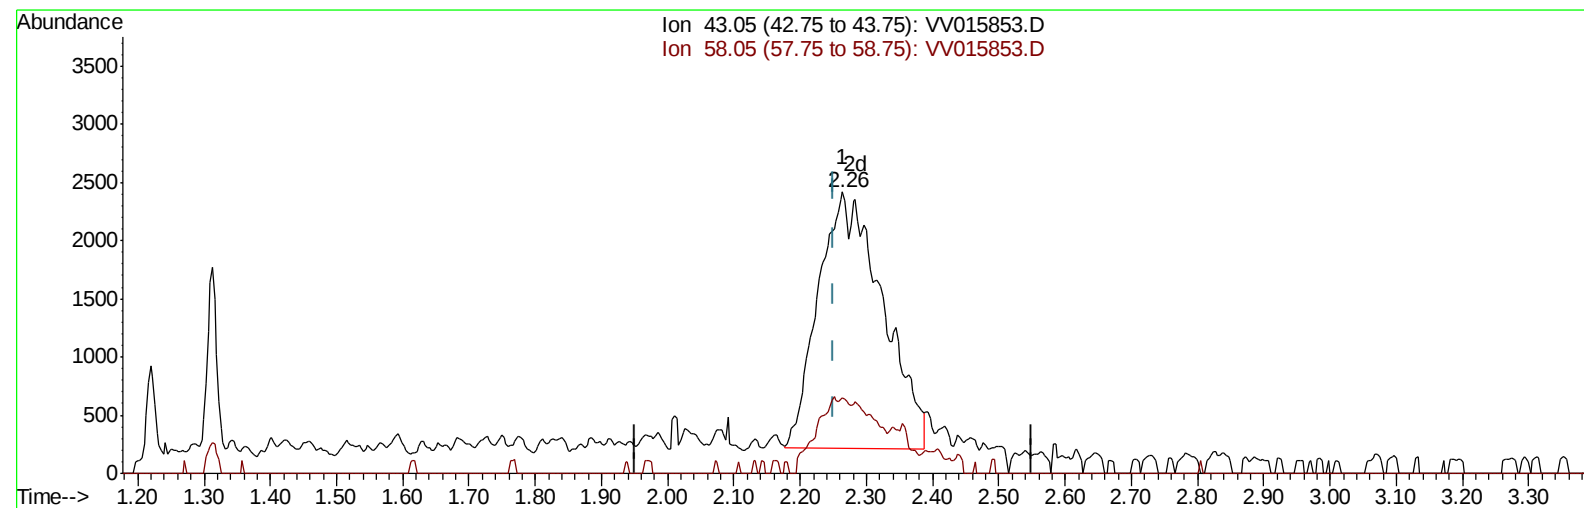

TIC: VV015853.D

(13) Acetone (T)

2.264min (+0.013) 11.45ug/L m

response 14829

Ion	Exp%	Act%
43.05	100	100
58.05	28.80	10.39
0.00	0.00	0.00
0.00	0.00	0.00