

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV050120\
 Data File : VV015856.D
 Acq On : 01 May 2020 13:47
 Operator : SY/MD
 Sample : VIBLK45
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK45

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M

Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	60	69	78	rBV	55966	59520	13.65%	1.631%
2	1.576	143	151	163	rBV	50872	59823	13.72%	1.640%
3	2.116	310	319	332	rVB	88900	127149	29.17%	3.485%
4	2.527	433	447	456	rBV2	4803	9501	2.18%	0.260%
5	3.968	879	895	940	rBV2	29506	167489	38.42%	4.591%
6	4.380	1006	1023	1054	rVB	66367	178038	40.84%	4.880%
7	5.074	1222	1239	1262	rBV2	161698	398275	91.37%	10.916%
8	5.643	1403	1416	1438	rBV	157292	319646	73.33%	8.761%
9	5.929	1497	1505	1517	rBV8	2217	4484	1.03%	0.123%
10	6.096	1544	1557	1583	rBV	93745	195825	44.92%	5.367%
11	7.013	1827	1842	1865	rBV	44855	85549	19.63%	2.345%
12	7.338	1930	1943	1963	rBV	184022	330130	75.74%	9.048%
13	7.646	2029	2039	2053	rBV2	26404	46722	10.72%	1.281%
14	8.116	2173	2185	2216	rBV	212720	435898	100.00%	11.947%
15	8.874	2409	2421	2449	rBV	245234	404315	92.75%	11.082%
16	10.241	2835	2846	2861	rBV	65508	104895	24.06%	2.875%
17	11.270	3154	3166	3184	rBV	251566	391351	89.78%	10.726%
18	11.646	3271	3283	3301	rBV	190920	306102	70.22%	8.390%
19	12.273	3468	3478	3488	rVB2	3535	5841	1.34%	0.160%
20	13.530	3856	3869	3877	rBV2	7704	13471	3.09%	0.369%
21	13.694	3910	3920	3930	rVB6	2302	4459	1.02%	0.122%


Sum of corrected areas: 3648483

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV050120\
Data File : VV015856.D
Acq On : 01 May 2020 13:47
Operator : SY/MD
Sample : VIBLK45
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

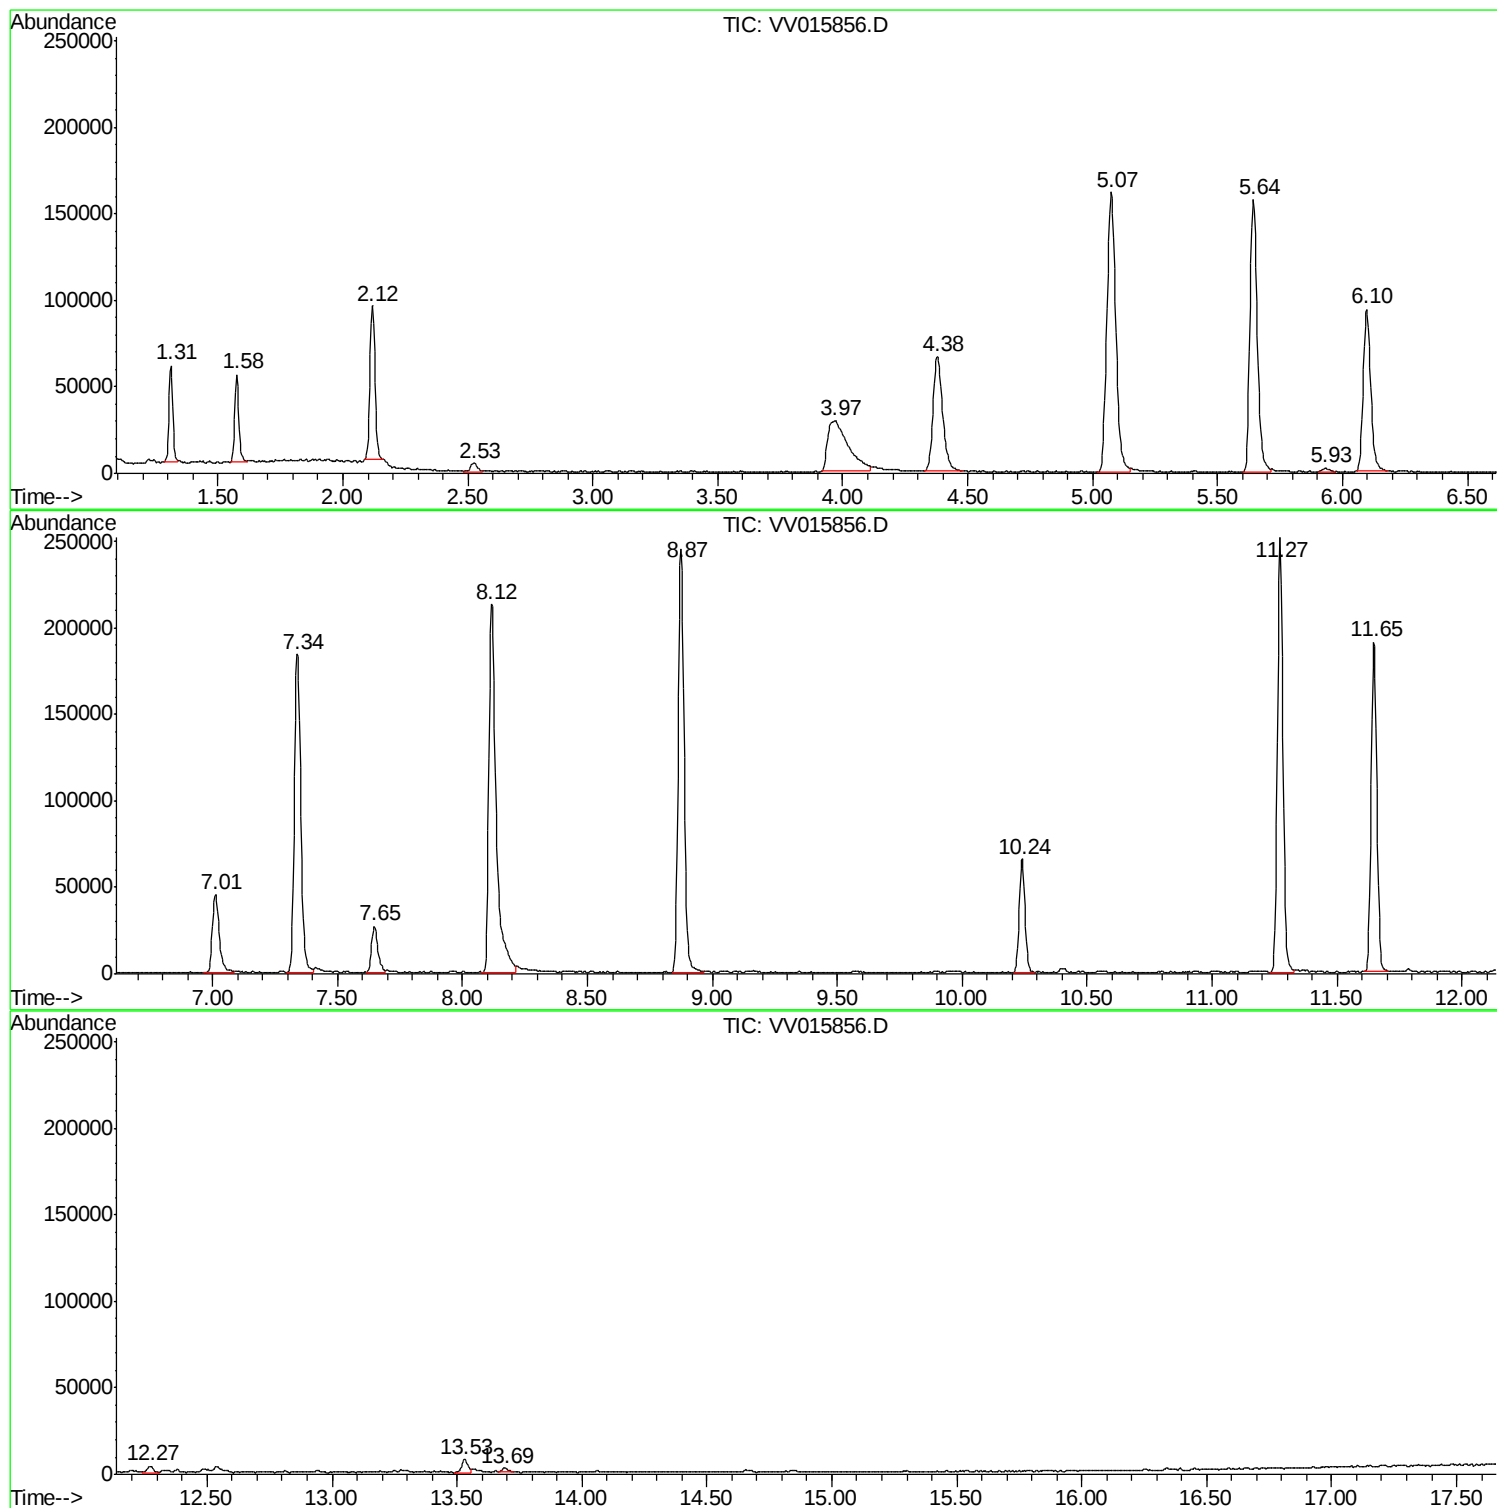

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV050120\
Data File : VV015856.D
Acq On : 01 May 2020 13:47
Operator : SY/MD
Sample : VIBLK45
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV050120\
Data File : VV015856.D
Acq On : 01 May 2020 13:47
Operator : SY/MD
Sample : VIBLK45
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc