


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV050120\
 Data File : VV015850.D
 Acq On : 01 May 2020 10:48
 Operator : SY/MD
 Sample : BFB48
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB48

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon May 04 05:01:15 2020

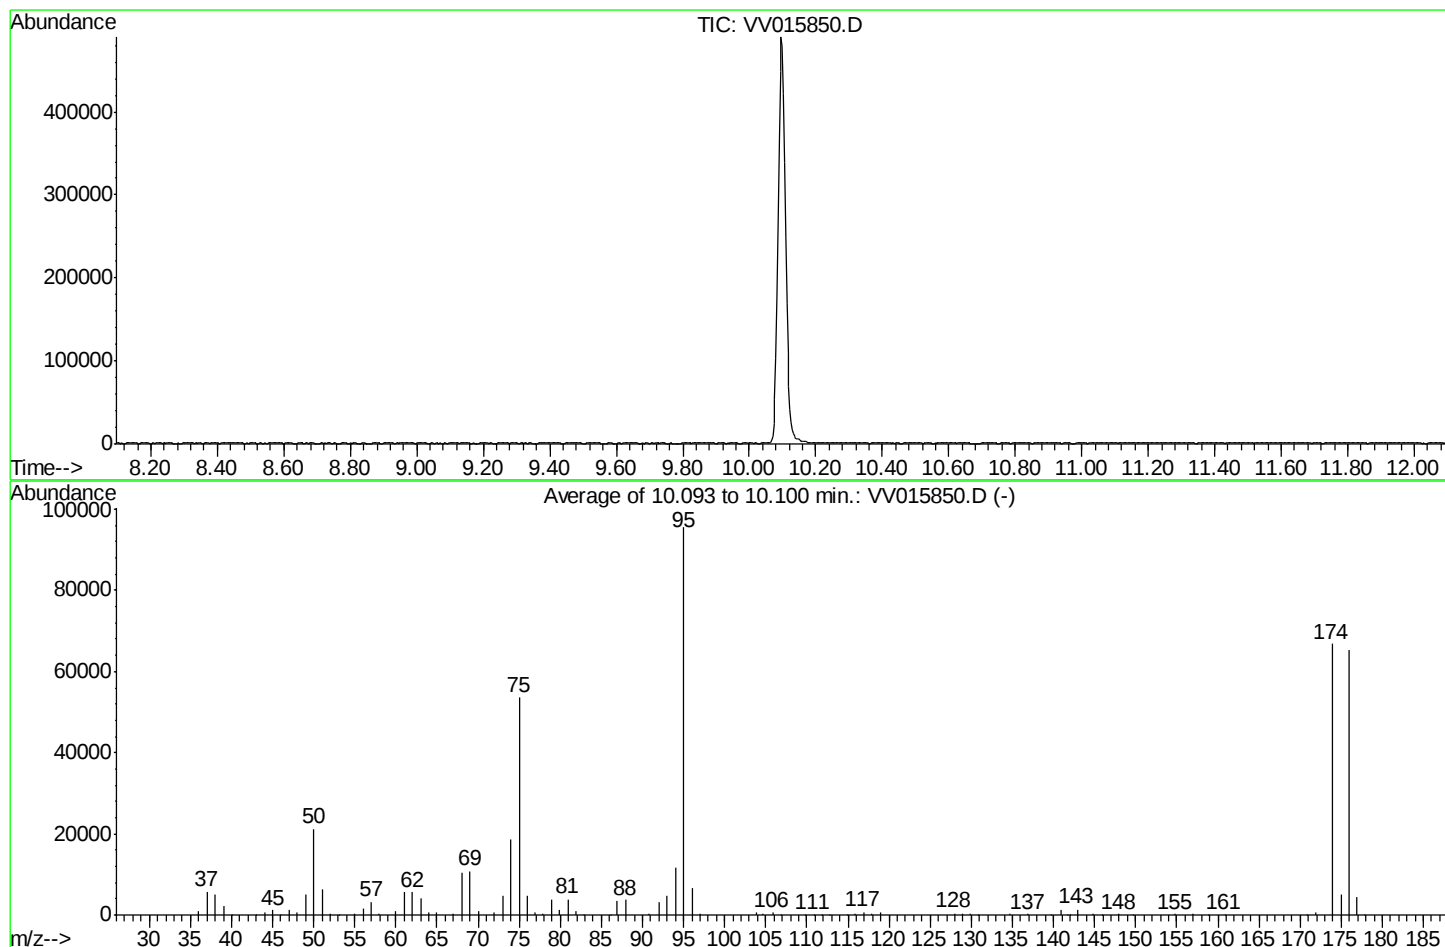

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	21269	PASS
75	95	30	80	56.0	53488	PASS
95	95	100	100	100.0	95546	PASS
96	95	5	9	7.0	6661	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	69.9	66792	PASS
175	174	5	9	7.8	5188	PASS
176	174	95	101	97.9	65421	PASS
177	176	5	9	6.7	4387	PASS

m/z	Abundance
36.00	1071.0
37.00	5556.0
38.00	4734.0
39.00	2163.0
40.00	483.0
43.00	145.0
44.00	1156.0
45.00	1111.0
46.00	119.0
47.00	1319.0
47.90	708.0
49.00	4690.0
50.00	20856.0
51.00	6014.0
52.00	318.0
54.90	434.0
56.00	1632.0
57.00	3087.0
57.90	191.0
60.00	927.0
61.00	5335.0
62.00	5349.0
63.00	4090.0
64.00	612.0
64.90	613.0
66.90	306.0
68.00	10155.0
69.00	10485.0
70.00	889.0
71.90	580.0
73.00	4524.0
74.00	17936.0
75.00	51496.0
76.00	4460.0
76.90	649.0
77.90	373.0
78.90	3502.0
79.90	1252.0
80.90	3782.0
81.90	855.0
86.90	3403.0
87.90	3642.0
90.90	376.0
91.90	2864.0
93.00	4277.0
94.00	11019.0
95.00	91032.0
96.00	6564.0
97.00	187.0
103.90	551.0
104.70	224.0
105.80	478.0
106.80	139.0
110.80	136.0
111.70	112.0
112.80	151.0
114.90	178.0
115.80	435.0
116.90	618.0
117.80	431.0
118.90	594.0
127.90	422.0
129.00	202.0
129.90	387.0
130.80	117.0
134.70	166.0
136.90	231.0
139.70	101.0
140.90	1216.0
142.00	114.0
142.90	1342.0
144.80	236.0
148.00	187.0
149.70	115.0
154.80	276.0
156.90	189.0
159.00	102.0
160.80	128.0
171.80	661.0
173.90	62168.0
175.00	4817.0
175.90	60112.0
176.90	4172.0
177.80	161.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.00	1143.0
37.00	6042.0
38.00	5112.0
39.00	2238.0
40.00	463.0
43.00	159.0
44.00	1091.0
45.00	1258.0
46.10	112.0
47.00	1355.0
47.90	762.0
49.00	5120.0
50.00	22064.0
51.00	6637.0
52.00	345.0
53.10	109.0
54.90	429.0
56.00	1766.0
57.00	3292.0
57.90	180.0
60.00	1045.0
61.00	5771.0
62.00	5811.0
63.00	4370.0
64.00	663.0
65.00	631.0
67.00	360.0
68.00	10878.0
69.00	11148.0
70.00	981.0
71.90	693.0
73.00	4902.0
74.00	19248.0
75.00	55744.0
76.00	4780.0
77.00	671.0
77.80	369.0
78.90	3823.0
80.00	1277.0
80.90	3966.0
81.90	989.0
82.90	118.0
86.90	3656.0
88.00	3902.0
90.80	435.0
91.90	3199.0
93.00	4891.0
94.00	11864.0
95.00	99120.0
96.00	6935.0
97.00	202.0
103.90	546.0
104.70	172.0
105.80	571.0
106.80	140.0
109.80	105.0
110.80	152.0
111.80	132.0
112.80	161.0
114.90	147.0
115.80	480.0
116.90	760.0
117.80	458.0
118.90	625.0
128.00	498.0
128.90	229.0
129.80	408.0
130.70	129.0
134.70	174.0
136.90	236.0
139.70	122.0
140.90	1287.0
141.70	112.0
142.90	1372.0
144.90	265.0
145.90	104.0
148.00	195.0
149.70	125.0
154.80	246.0
156.90	178.0
158.80	113.0
160.80	180.0
170.80	111.0
171.90	824.0
173.90	69056.0
175.00	5409.0
175.90	67624.0
176.90	4522.0
177.80	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.00	1104.0
37.00	5869.0
38.00	5033.0
39.00	2121.0
40.00	477.0
43.00	137.0
44.00	966.0
45.00	1163.0
45.90	121.0
47.00	1251.0
47.90	689.0
49.00	5009.0
50.00	20888.0
51.00	6569.0
52.00	306.0
53.10	130.0
54.90	370.0
56.00	1807.0
57.00	3147.0
58.00	164.0
60.00	1073.0
61.00	5574.0
62.00	5583.0
63.00	4091.0
64.10	635.0
65.00	610.0
67.00	388.0
68.00	10589.0
69.00	10833.0
70.00	966.0
72.00	711.0
73.00	4805.0
74.00	18480.0
75.00	53224.0
76.00	4634.0
77.00	625.0
77.70	385.0
78.90	3837.0
80.00	1215.0
80.90	3801.0
81.90	967.0
82.80	137.0
86.10	128.0
87.00	3509.0
88.00	3690.0
90.80	471.0
92.00	3214.0
93.00	4862.0
94.00	11740.0
95.00	96488.0
96.00	6486.0
96.90	199.0
103.90	485.0
104.60	131.0
105.90	596.0
106.60	133.0
109.80	104.0
110.90	136.0
111.80	150.0
112.80	147.0
115.00	111.0
115.80	453.0
116.90	777.0
117.80	436.0
118.90	606.0
128.00	473.0
128.90	244.0
129.80	414.0
130.70	163.0
134.70	174.0
136.90	210.0
139.70	132.0
140.90	1216.0
141.70	133.0
142.90	1219.0
144.90	280.0
145.90	116.0
147.90	180.0
154.80	224.0
156.90	170.0
158.80	146.0
160.80	166.0
171.90	826.0
173.90	69152.0
175.00	5338.0
175.90	68528.0
176.90	4468.0
177.80	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

Scan 2788 (10.055 min): VV015850.D
BFB48

m/z	Abundance
39.90	363.0
44.00	494.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48