




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
 Data File : VV030947.D
 Acq On : 01 May 2023 11:48
 Operator : SY/MD
 Sample : 02528-02 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 HOA34

Manual IntegrationsAPPROVED

Quant Time: May 02 01:33:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 29 01:06:38 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

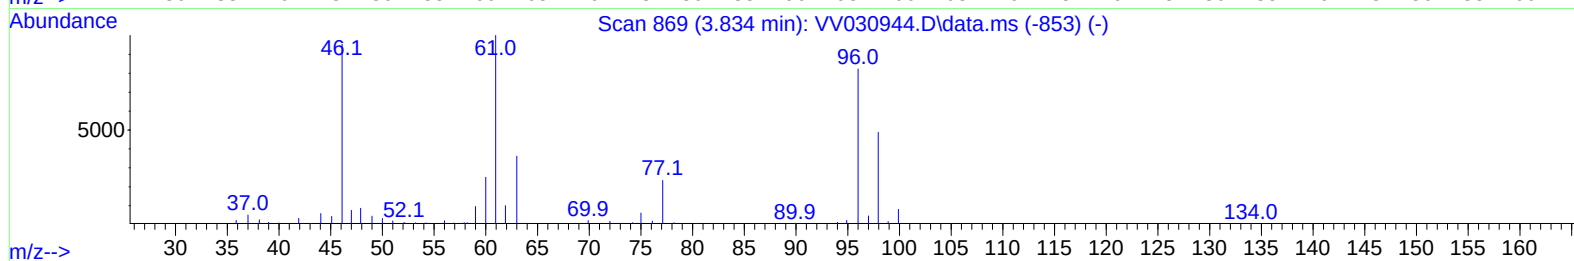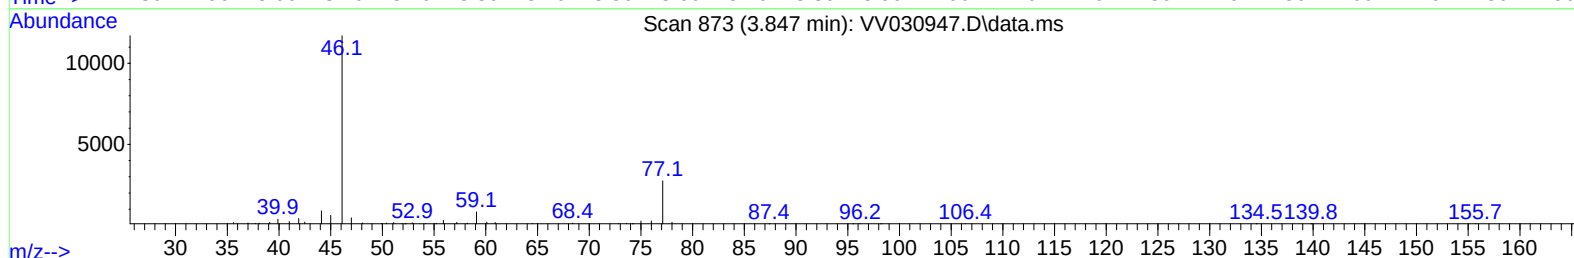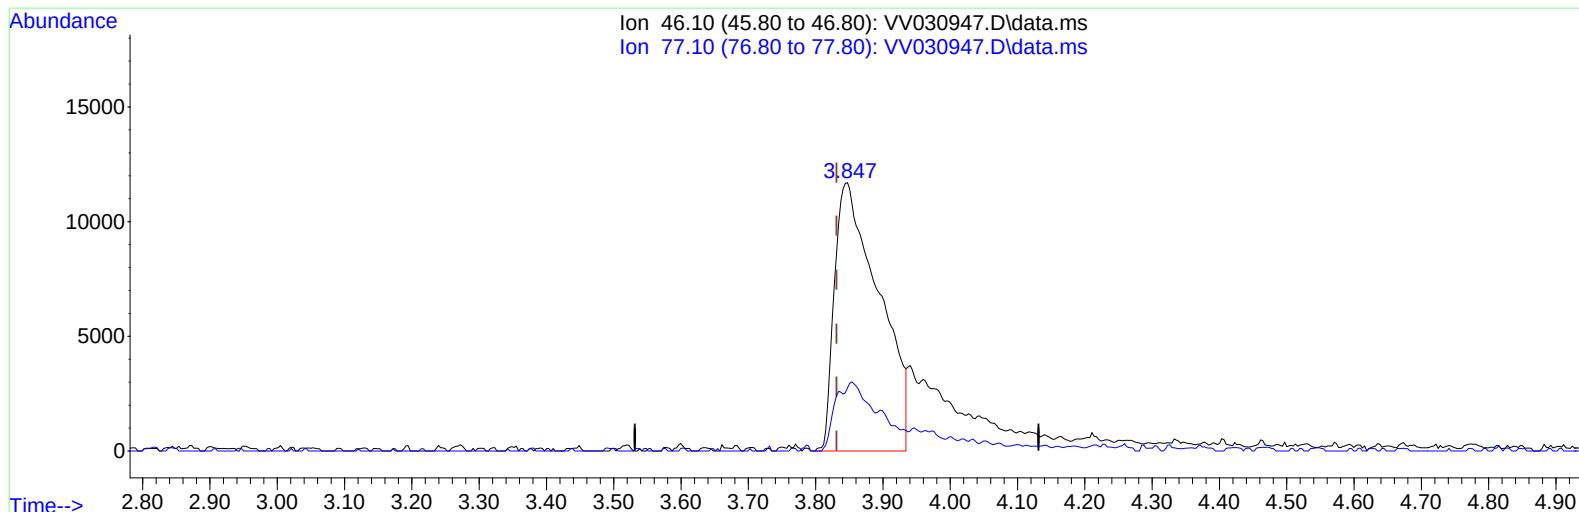

TIC: VV030947.D\data.ms

(20) 2-Butanone-d5 (S)

3.847min (+ 0.016) 31.25 ug/L

response 53633

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	7.40	5.41
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
 Data File : VV030947.D
 Acq On : 01 May 2023 11:48
 Operator : SY/MD
 Sample : 02528-02 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 HOA34

Manual IntegrationsAPPROVED

Quant Time: May 02 01:33:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 29 01:06:38 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

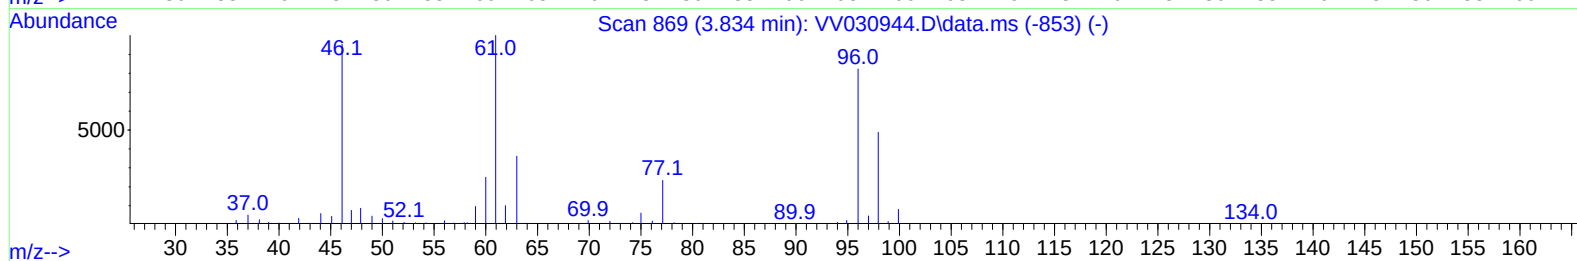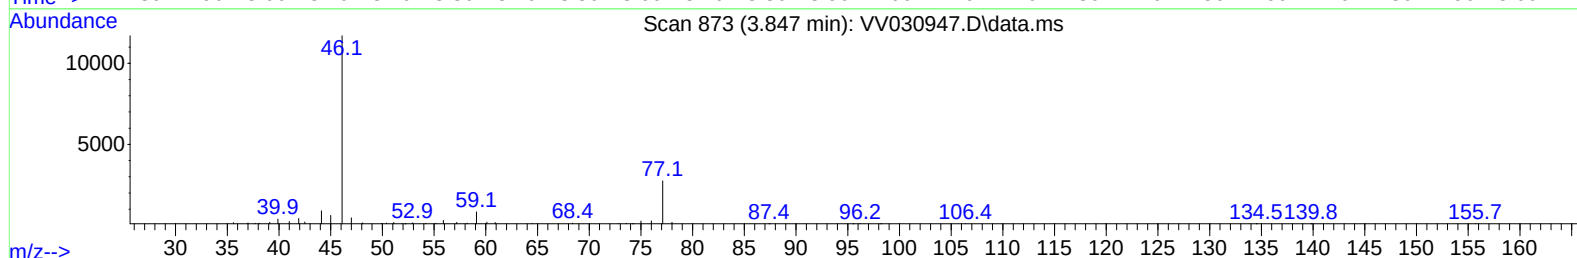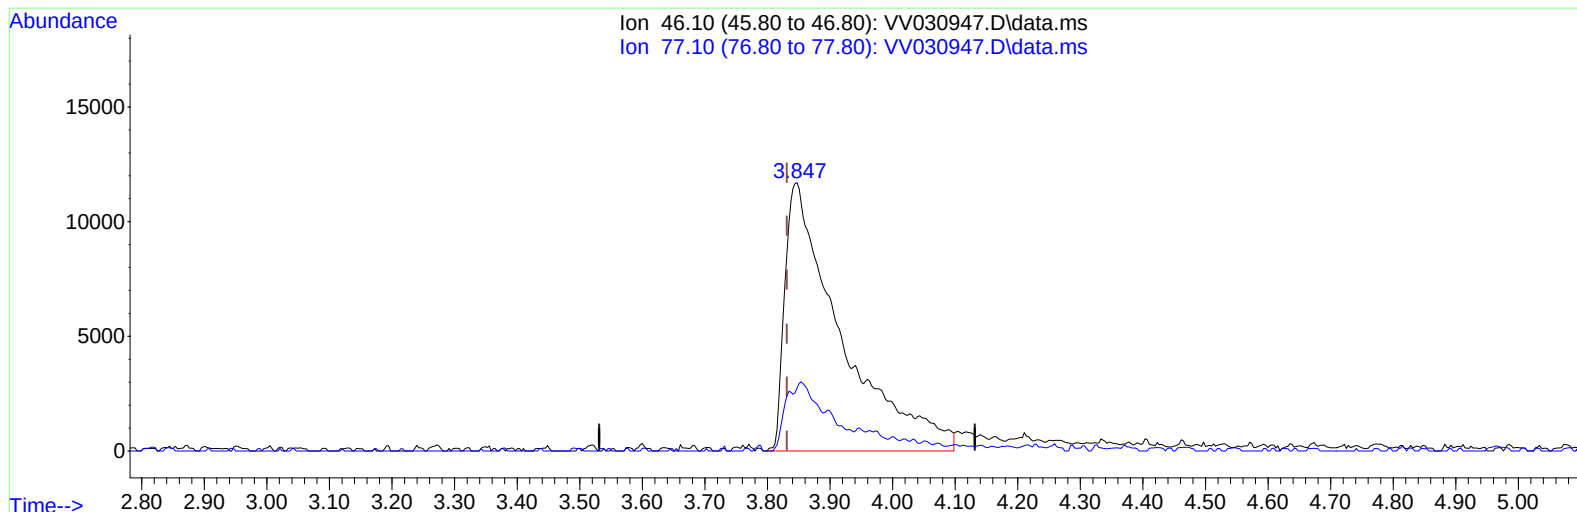

TIC: VV030947.D\data.ms

(20) 2-Butanone-d5 (S)

3.847min (+ 0.016) 42.29 ug/L m

response 72579

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	7.40	3.99#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
 Data File : VV030947.D
 Acq On : 01 May 2023 11:48
 Operator : SY/MD
 Sample : 02528-02 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 HOA34

Manual IntegrationsAPPROVED

Quant Time: May 02 01:33:03 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 29 01:06:38 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 05/02/2023
 Supervised By :Mahesh Dadoda 05/02/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	117455	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	116570	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	60961	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	46037	4.757	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	95.200%	
7) Chloroethane-d5	1.535	69	37629	4.767	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.400%	
11) 1,1-Dichloroethene-d2	2.063	65	23641	4.616	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	92.400%	
20) 2-Butanone-d5	3.847	46	72579m	42.295	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	84.580%	
24) Chloroform-d	4.259	84	83894	4.362	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.200%	
26) 1,2-Dichloroethane-d4	4.953	65	42738	4.371	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.400%	
32) Benzene-d6	4.969	84	144018	4.215	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.200%	
36) 1,2-Dichloropropane-d6	5.998	67	42268	4.254	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	85.000%	
41) Toluene-d8	7.252	98	129484	3.979	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	79.600%	
43) trans-1,3-Dichloroprop...	7.564	79	15783	4.238	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	84.800%	
46) 2-Hexanone-d5	8.040	63	51595	39.540	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	79.080%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84	29386	4.080	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	81.600%	
66) 1,2-Dichlorobenzene-d4	11.570	152	49645	4.369	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	87.400%	
Target Compounds						
12) 1,1-Dichloroethene	2.072	96	5682	0.719	ug/L #	1
34) Trichloroethene	5.844	95	13380	1.712	ug/L	98
47) Tetrachloroethene	7.911	164	104557	14.022	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030947.D
Acq On : 01 May 2023 11:48
Operator : SY/MD
Sample : 02528-02 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA34

Manual IntegrationsAPPROVED

Quant Time: May 02 01:33:03 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 29 01:06:38 2023
Response via : Initial Calibration

Reviewed By :John Carlone 05/02/2023
Supervised By :Mahesh Dadoda 05/02/2023

