

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
 Data File : VV030945.D
 Acq On : 01 May 2023 10:59
 Operator : SY/MD
 Sample : VV0501WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK331

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030945.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	87	rVB	68491	77775	17.26%	2.107%
2	1.535	146	154	168	rBV	61739	74302	16.49%	2.013%
3	2.063	309	318	332	rBV	145796	206941	45.92%	5.607%
4	2.452	431	439	447	rBV4	10022	17507	3.89%	0.474%
5	3.844	860	872	891	rBV2	23017	93157	20.67%	2.524%
6	4.259	985	1001	1021	rBV2	80404	210150	46.64%	5.694%
7	4.966	1200	1221	1244	rBV3	173072	450611	100.00%	12.209%
8	5.542	1389	1400	1420	rBV	143352	302704	67.18%	8.202%
9	5.998	1529	1542	1561	rBV2	102384	219606	48.74%	5.950%
10	6.924	1820	1830	1844	rBV2	42956	83169	18.46%	2.253%
11	7.252	1919	1932	1949	rBV	197985	362310	80.40%	9.817%
12	7.564	2017	2029	2045	rBV2	26781	52730	11.70%	1.429%
13	8.040	2165	2177	2210	rBV	128232	325396	72.21%	8.817%
14	8.792	2396	2411	2431	rBV	225549	393443	87.31%	10.660%
15	10.162	2825	2837	2854	rVB2	71361	119899	26.61%	3.249%
16	11.194	3145	3158	3177	rBV	227905	371172	82.37%	10.057%
17	11.570	3262	3275	3293	rBV	191459	315282	69.97%	8.542%
18	13.220	3777	3788	3791	rBV	3723	6228	1.38%	0.169%
19	13.458	3853	3862	3872	rVB10	4091	8375	1.86%	0.227%




Sum of corrected areas: 3690757

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030945.D
Acq On : 01 May 2023 10:59
Operator : SY/MD
Sample : VV0501WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK331

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

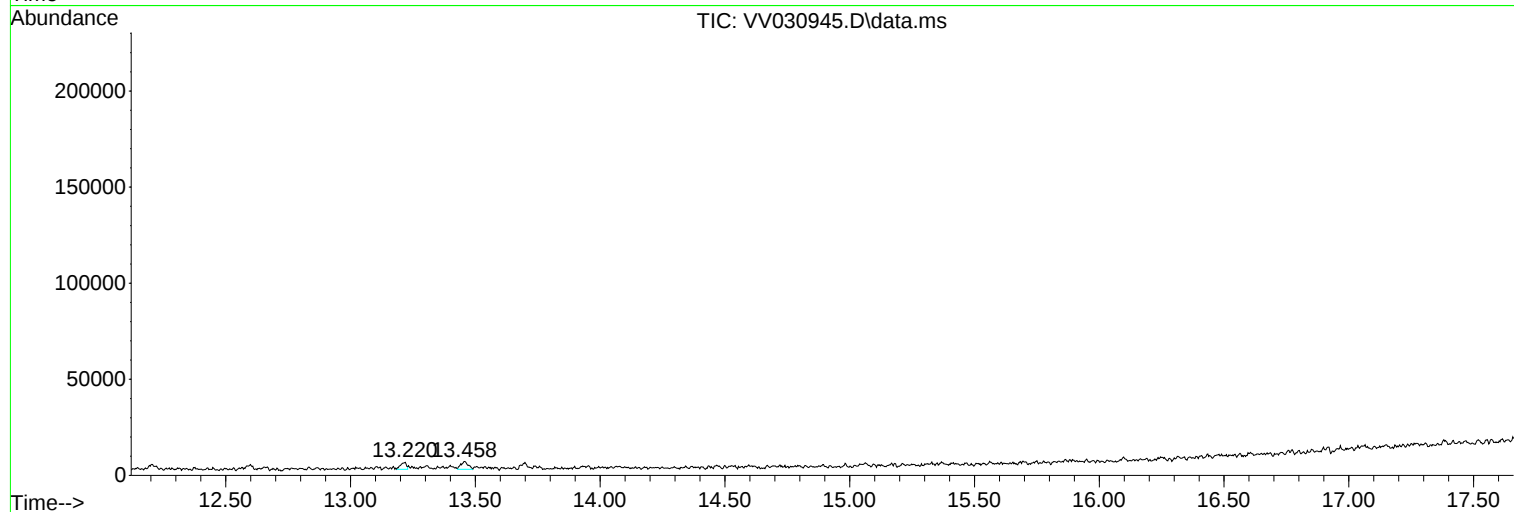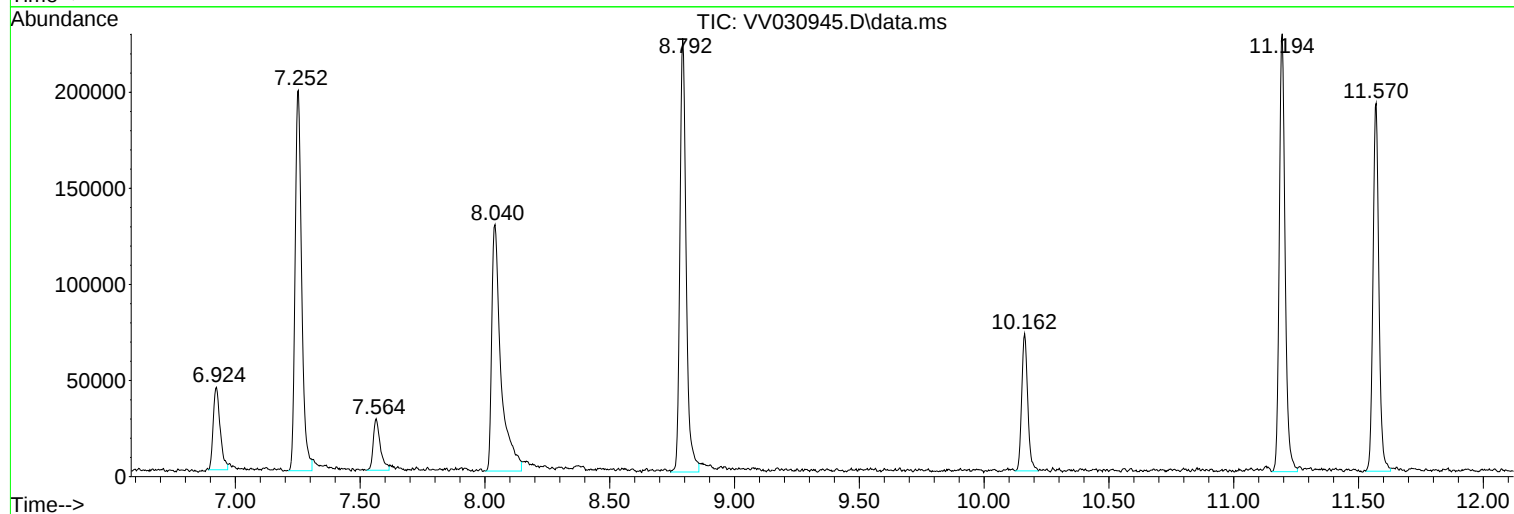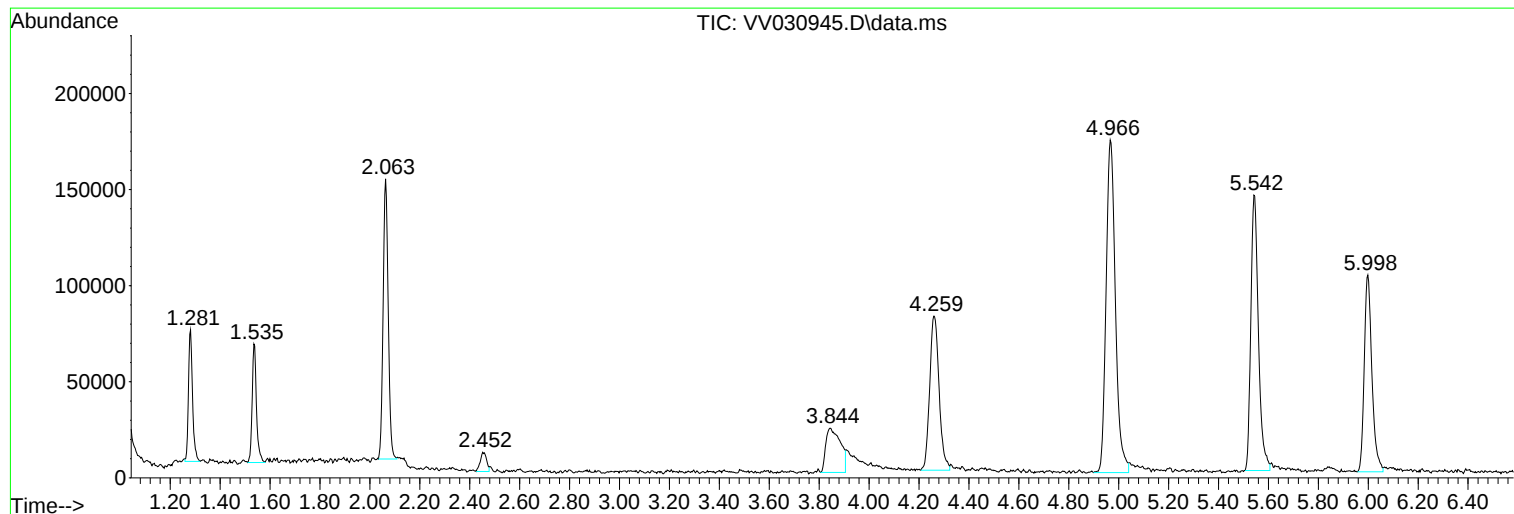

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030945.D
Acq On : 01 May 2023 10:59
Operator : SY/MD
Sample : VV0501WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK331

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030945.D
Acq On : 01 May 2023 10:59
Operator : SY/MD
Sample : VV0501WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK331

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------