

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
 Data File : VV030946.D
 Acq On : 01 May 2023 11:23
 Operator : SY/MD
 Sample : 02528-01 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 HOA33

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	90	rVB	71504	80186	17.46%	1.923%
2	1.535	146	154	167	rBV	60577	75944	16.54%	1.821%
3	2.063	307	318	333	rBV	147317	221218	48.18%	5.304%
4	3.841	860	871	872	rBV	22170	30092	6.55%	0.722%
5	4.259	986	1001	1021	rBV2	86481	216121	47.07%	5.182%
6	4.526	1076	1084	1091	rVB9	5606	8341	1.82%	0.200%
7	4.969	1204	1222	1243	rBV2	179073	459149	100.00%	11.010%
8	5.542	1385	1400	1417	rBV2	152420	323373	70.43%	7.754%
9	5.847	1486	1495	1505	rBV2	9495	21412	4.66%	0.513%
10	5.998	1526	1542	1562	rBV2	102273	222724	48.51%	5.341%
11	6.921	1819	1829	1848	rBV2	45716	87271	19.01%	2.093%
12	7.252	1917	1932	1949	rBV	202629	367752	80.09%	8.818%
13	7.564	2018	2029	2049	rBV2	27734	56614	12.33%	1.358%
14	7.911	2125	2137	2151	rBV	240502	413078	89.97%	9.905%
15	8.040	2167	2177	2214	rBV	138425	335368	73.04%	8.042%
16	8.792	2400	2411	2429	rBV	239970	407237	88.69%	9.765%
17	10.162	2823	2837	2859	rBV	74567	128302	27.94%	3.077%
18	11.194	3146	3158	3177	rBV	240063	390641	85.08%	9.367%
19	11.570	3261	3275	3288	rBV	195034	325561	70.91%	7.806%




Sum of corrected areas: 4170384

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030946.D
Acq On : 01 May 2023 11:23
Operator : SY/MD
Sample : 02528-01 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

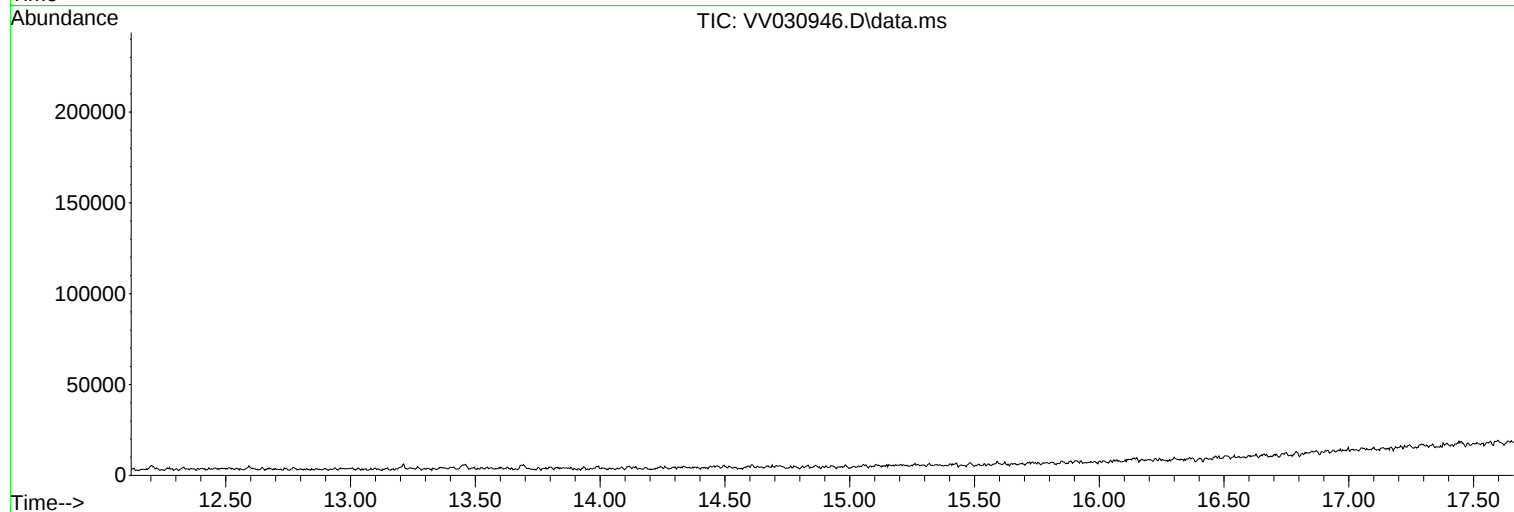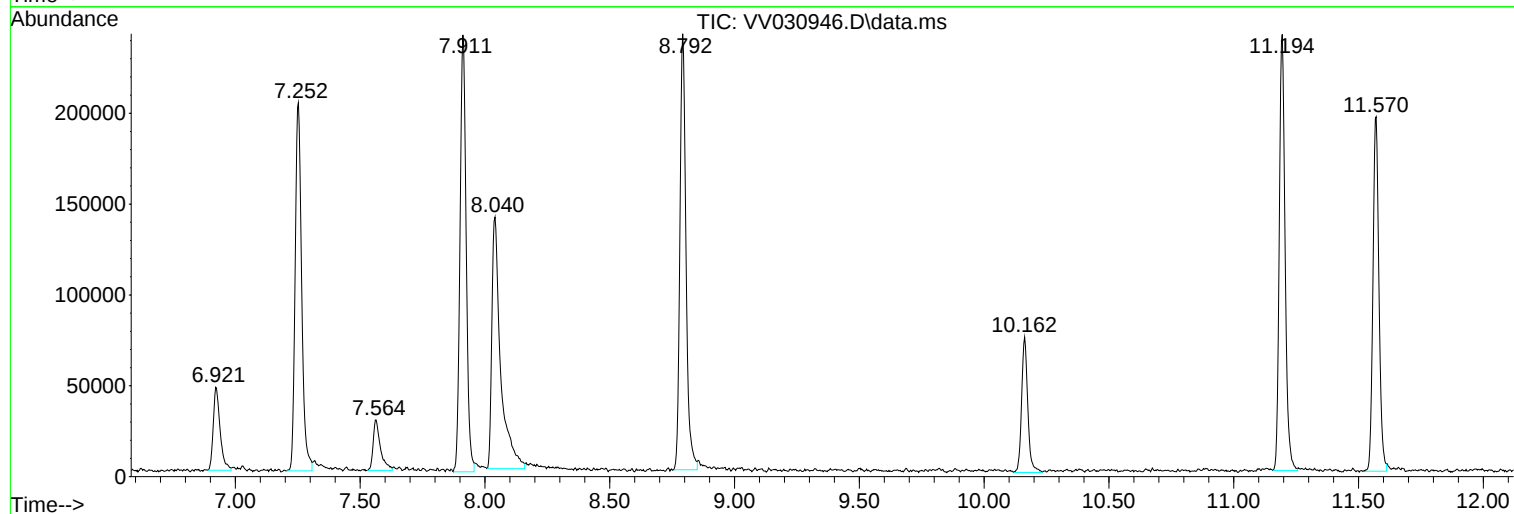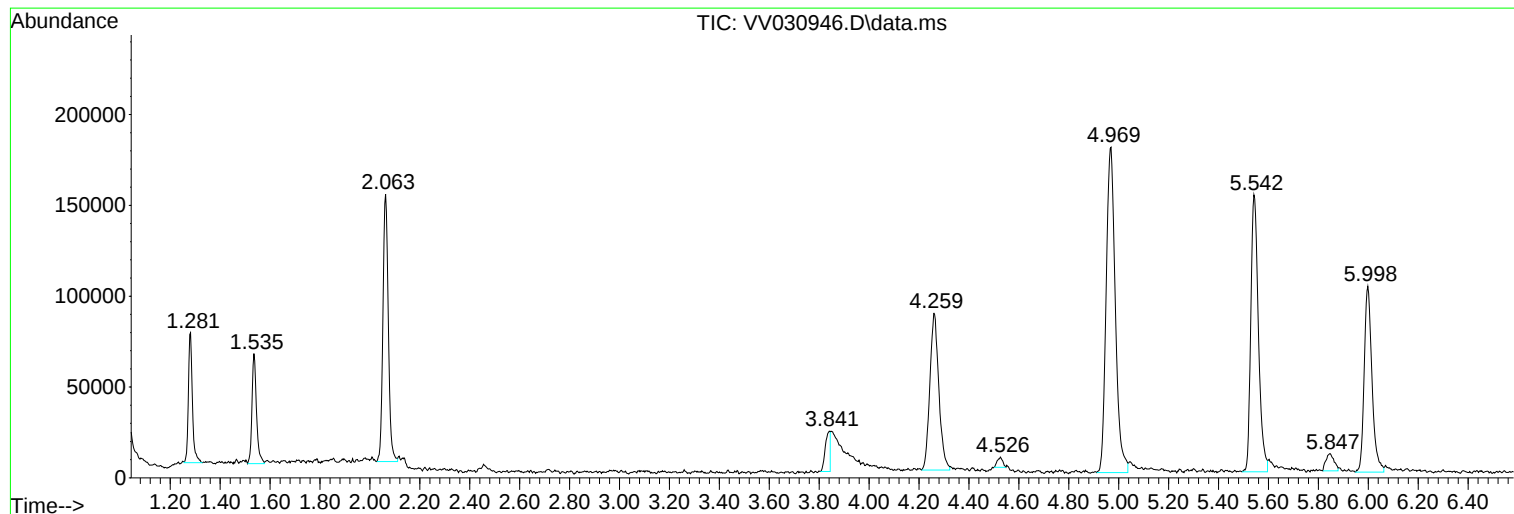

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030946.D
Acq On : 01 May 2023 11:23
Operator : SY/MD
Sample : 02528-01 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030946.D
Acq On : 01 May 2023 11:23
Operator : SY/MD
Sample : 02528-01 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc