

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
 Data File : VV030947.D
 Acq On : 01 May 2023 11:48
 Operator : SY/MD
 Sample : 02528-02 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 HOA34

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	64	74	88	rBV	69620	85347	10.44%	1.908%
2	1.535	145	154	164	rBV	55080	69114	8.45%	1.545%
3	2.063	309	318	342	rVB2	152336	253761	31.03%	5.672%
4	3.850	858	874	892	rBV2	21186	82820	10.13%	1.851%
5	4.262	984	1002	1026	rBV	81180	216856	26.52%	4.847%
6	4.966	1204	1221	1247	rBV2	167633	432178	52.85%	9.660%
7	5.542	1386	1400	1423	rBV2	137925	296658	36.28%	6.631%
8	5.844	1483	1494	1514	rVB3	38347	83808	10.25%	1.873%
9	5.998	1528	1542	1559	rBV2	99456	208759	25.53%	4.666%
10	6.924	1820	1830	1842	rBV2	40955	78057	9.55%	1.745%
11	7.252	1920	1932	1957	rBV	189939	354728	43.38%	7.929%
12	7.564	2017	2029	2039	rBV2	25677	47899	5.86%	1.071%
13	7.911	2122	2137	2156	rBV	475636	817758	100.00%	18.279%
14	8.040	2165	2177	2205	rBV2	131950	310144	37.93%	6.932%
15	8.792	2399	2411	2429	rBV	210693	365134	44.65%	8.162%
16	10.162	2825	2837	2859	rBV2	69044	117119	14.32%	2.618%
17	11.194	3146	3158	3175	rBV	214349	349115	42.69%	7.803%
18	11.567	3263	3274	3289	rBV	183744	304581	37.25%	6.808%




Sum of corrected areas: 4473836

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030947.D
Acq On : 01 May 2023 11:48
Operator : SY/MD
Sample : 02528-02 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

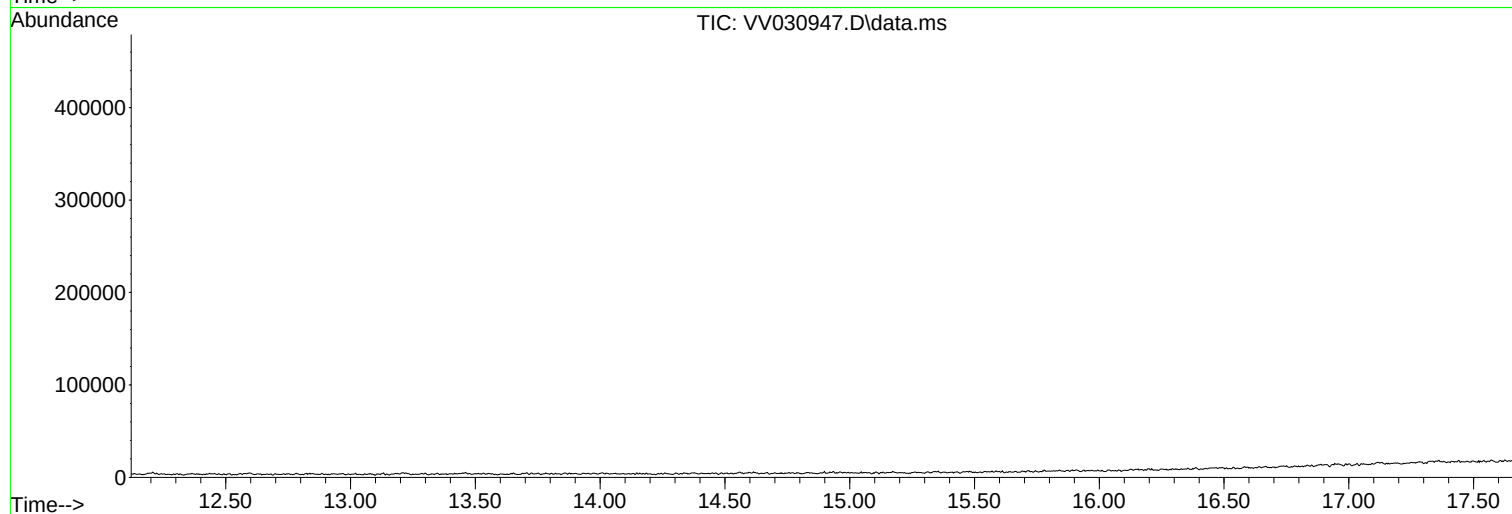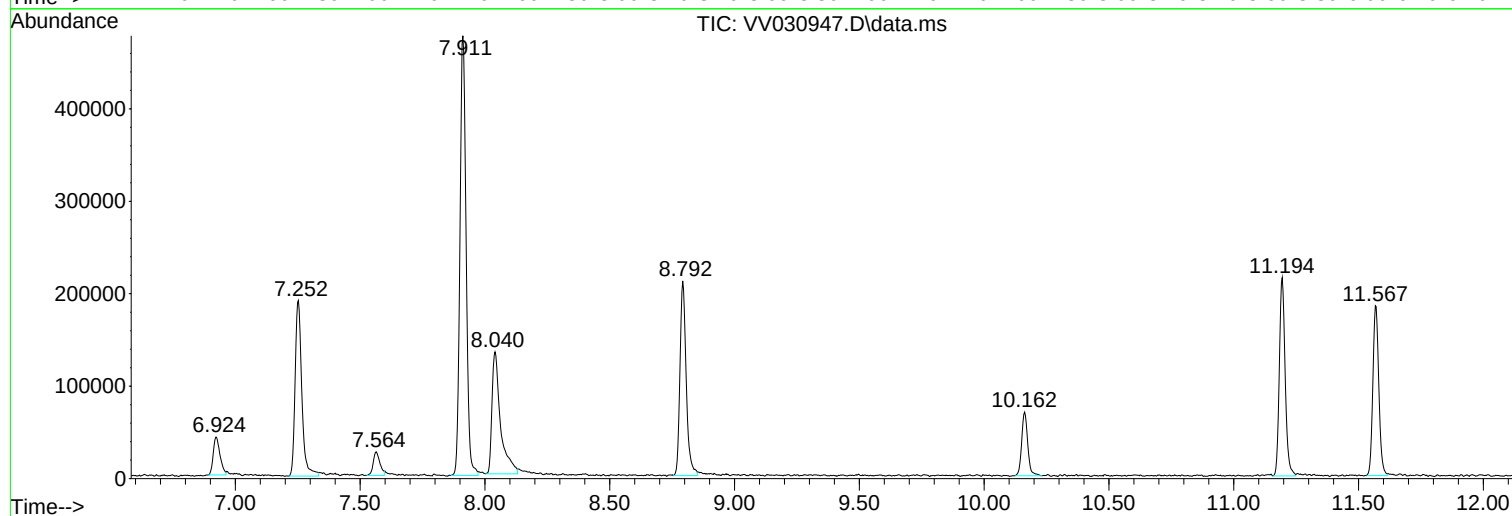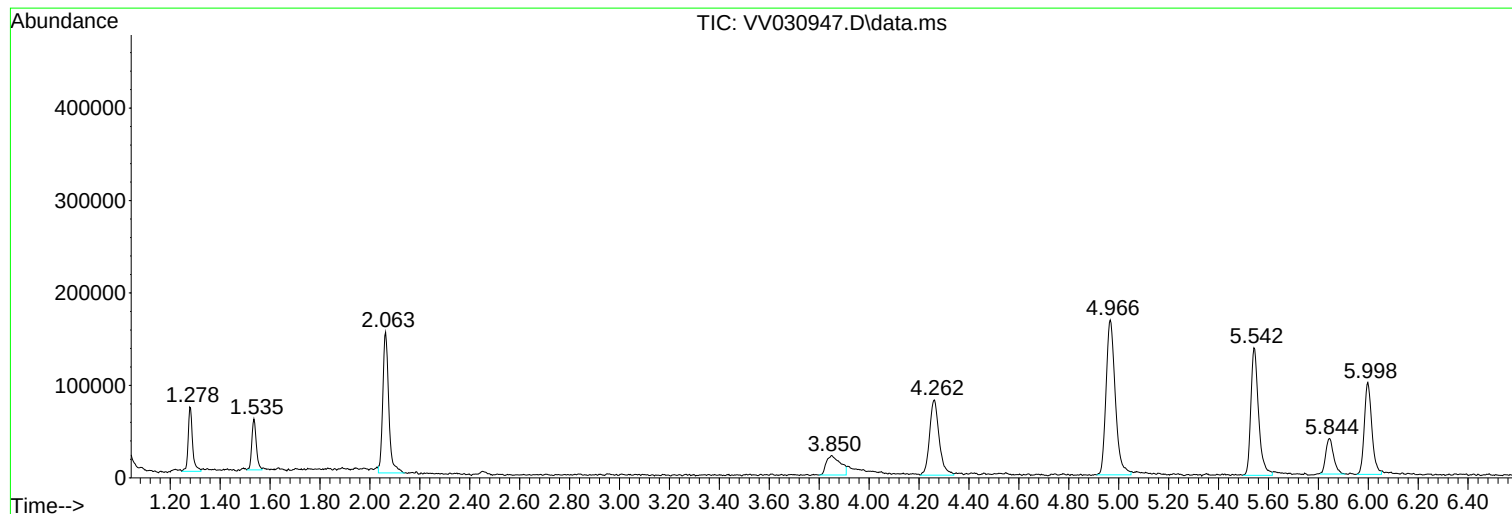

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030947.D
Acq On : 01 May 2023 11:48
Operator : SY/MD
Sample : 02528-02 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030947.D
Acq On : 01 May 2023 11:48
Operator : SY/MD
Sample : 02528-02 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA34

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------