

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
 Data File : VV030948.D
 Acq On : 01 May 2023 12:13
 Operator : SY/MD
 Sample : 02528-03 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 HOA35

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	85	rBV	63989	72076	9.47%	1.692%
2	1.535	147	154	170	rVB	54001	66346	8.71%	1.557%
3	2.063	308	318	332	rBV2	146485	225180	29.57%	5.285%
4	3.844	859	872	874	rBV2	19015	33220	4.36%	0.780%
5	4.262	985	1002	1021	rBV3	74562	194993	25.61%	4.577%
6	4.966	1204	1221	1247	rBV2	162561	422557	55.50%	9.918%
7	5.542	1387	1400	1421	rBV2	138413	300340	39.44%	7.049%
8	5.844	1482	1494	1510	rBV3	38938	82908	10.89%	1.946%
9	5.998	1528	1542	1560	rBV	94279	201634	26.48%	4.733%
10	6.921	1820	1829	1843	rBV2	40923	79381	10.43%	1.863%
11	7.252	1920	1932	1948	rBV	188025	334289	43.90%	7.846%
12	7.564	2018	2029	2040	rBV3	25163	46454	6.10%	1.090%
13	7.911	2124	2137	2159	rBV	439815	761421	100.00%	17.872%
14	8.040	2167	2177	2208	rBV	125250	298453	39.20%	7.005%
15	8.792	2399	2411	2429	rBV	218060	373244	49.02%	8.761%
16	10.162	2826	2837	2850	rBV2	67922	113273	14.88%	2.659%
17	11.194	3147	3158	3177	rBV	219755	355531	46.69%	8.345%
18	11.570	3263	3275	3291	rBV	182000	299226	39.30%	7.023%




Sum of corrected areas: 4260526

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030948.D
Acq On : 01 May 2023 12:13
Operator : SY/MD
Sample : 02528-03 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

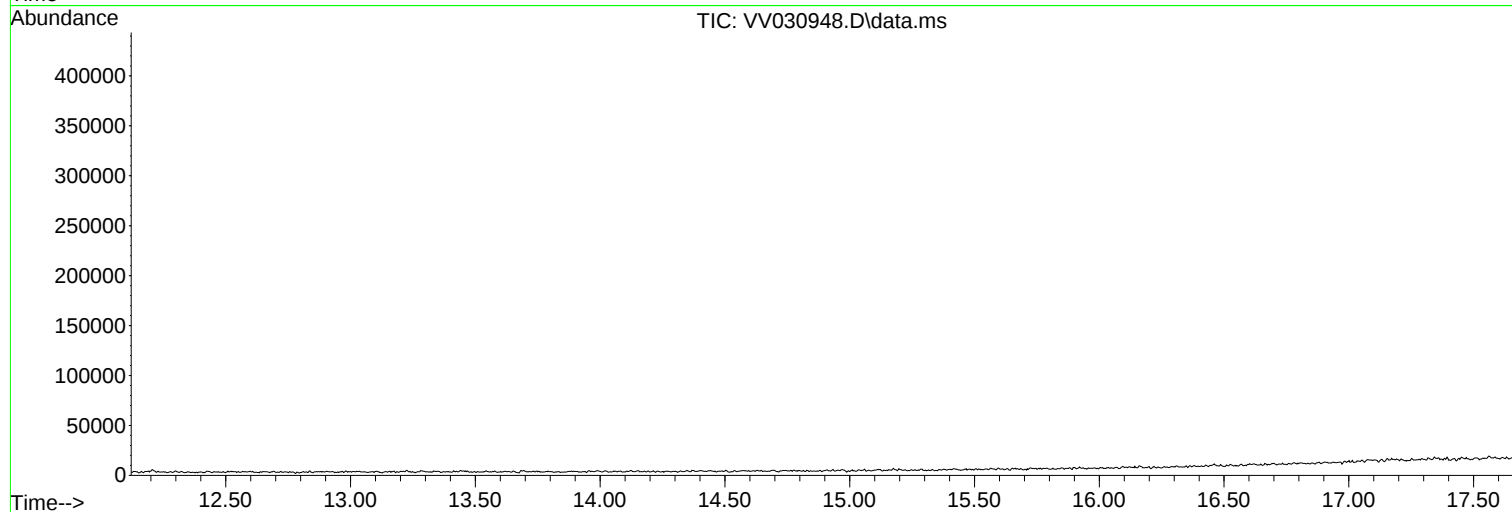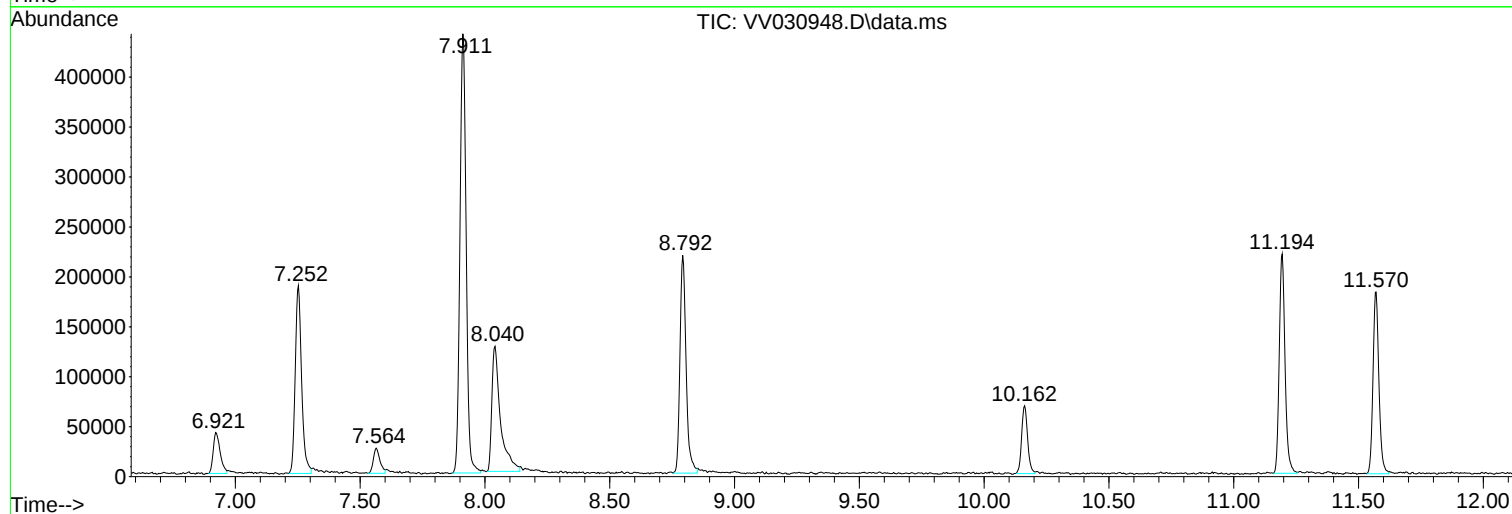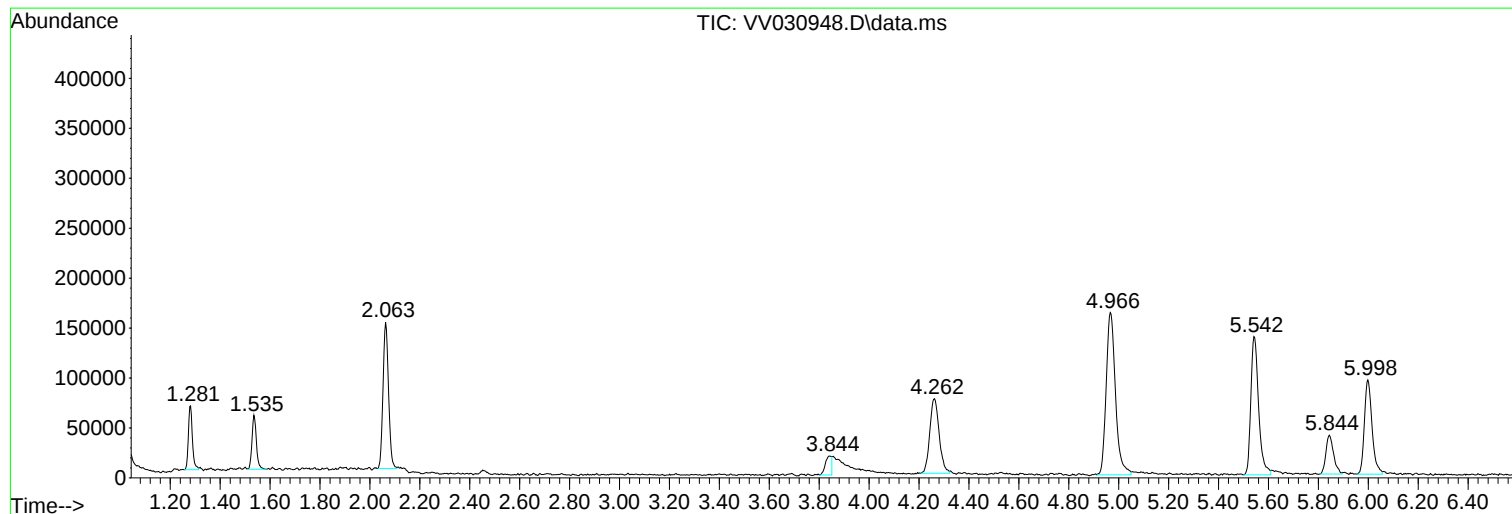

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030948.D
Acq On : 01 May 2023 12:13
Operator : SY/MD
Sample : 02528-03 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030948.D
Acq On : 01 May 2023 12:13
Operator : SY/MD
Sample : 02528-03 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------