

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
 Data File : VV030949.D
 Acq On : 01 May 2023 12:37
 Operator : SY/MD
 Sample : 02528-04 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 HOA36

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030949.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	84	rBV	70550	76745	17.00%	1.865%
2	1.536	147	154	165	rBV	59204	71292	15.79%	1.733%
3	2.063	308	318	335	rBV	144394	212610	47.10%	5.167%
4	2.455	427	440	447	rBV3	6571	13031	2.89%	0.317%
5	3.844	859	872	898	rBV	23728	109322	24.22%	2.657%
6	4.259	982	1001	1023	rBV	84631	225920	50.05%	5.491%
7	4.966	1202	1221	1251	rBV3	174817	451381	100.00%	10.970%
8	5.542	1385	1400	1421	rBV2	144058	311705	69.06%	7.576%
9	5.847	1481	1495	1508	rBV4	20841	44898	9.95%	1.091%
10	5.998	1530	1542	1560	rBV2	100119	214142	47.44%	5.205%
11	6.924	1818	1830	1846	rBV2	44093	87493	19.38%	2.126%
12	7.252	1919	1932	1953	rBV	200476	363562	80.54%	8.836%
13	7.564	2019	2029	2042	rBV2	27237	52745	11.69%	1.282%
14	7.911	2126	2137	2153	rBV	206308	354500	78.54%	8.616%
15	8.040	2167	2177	2206	rBV	139453	324143	71.81%	7.878%
16	8.371	2275	2280	2288	rVB9	4576	4915	1.09%	0.119%
17	8.792	2398	2411	2433	rBV	225484	387223	85.79%	9.411%
18	10.162	2825	2837	2855	rBV2	71720	119295	26.43%	2.899%
19	11.194	3147	3158	3183	rBV	224529	366181	81.12%	8.900%
20	11.567	3263	3274	3296	rBV	192474	323402	71.65%	7.860%




Sum of corrected areas: 4114505

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030949.D
Acq On : 01 May 2023 12:37
Operator : SY/MD
Sample : 02528-04 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

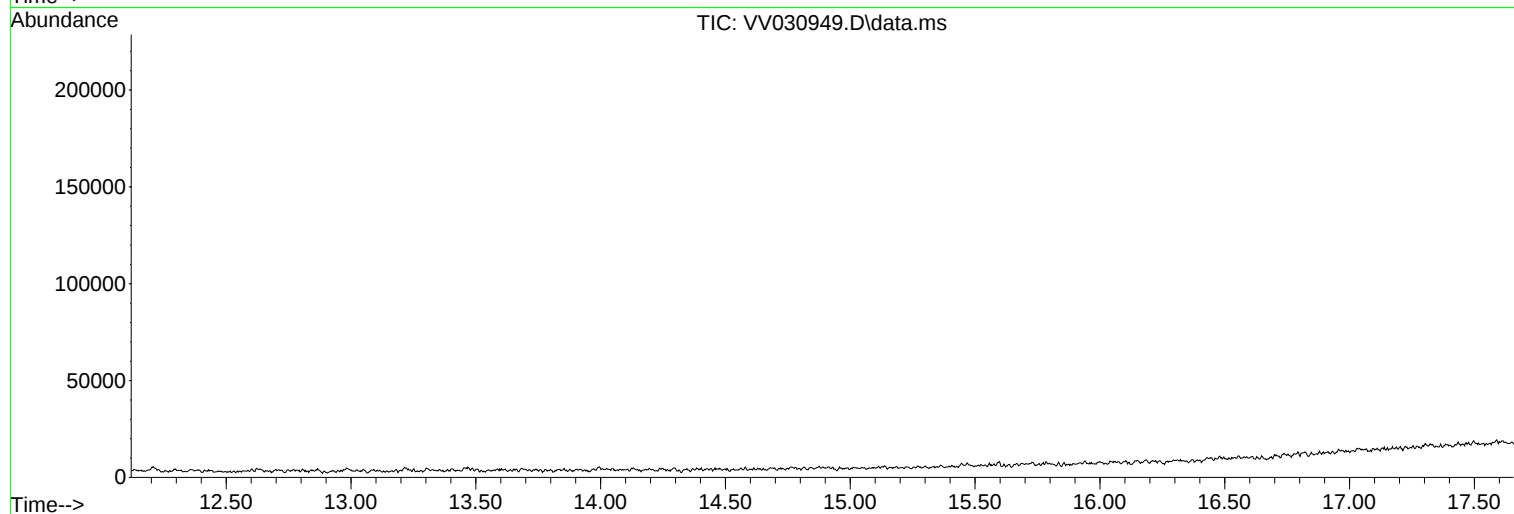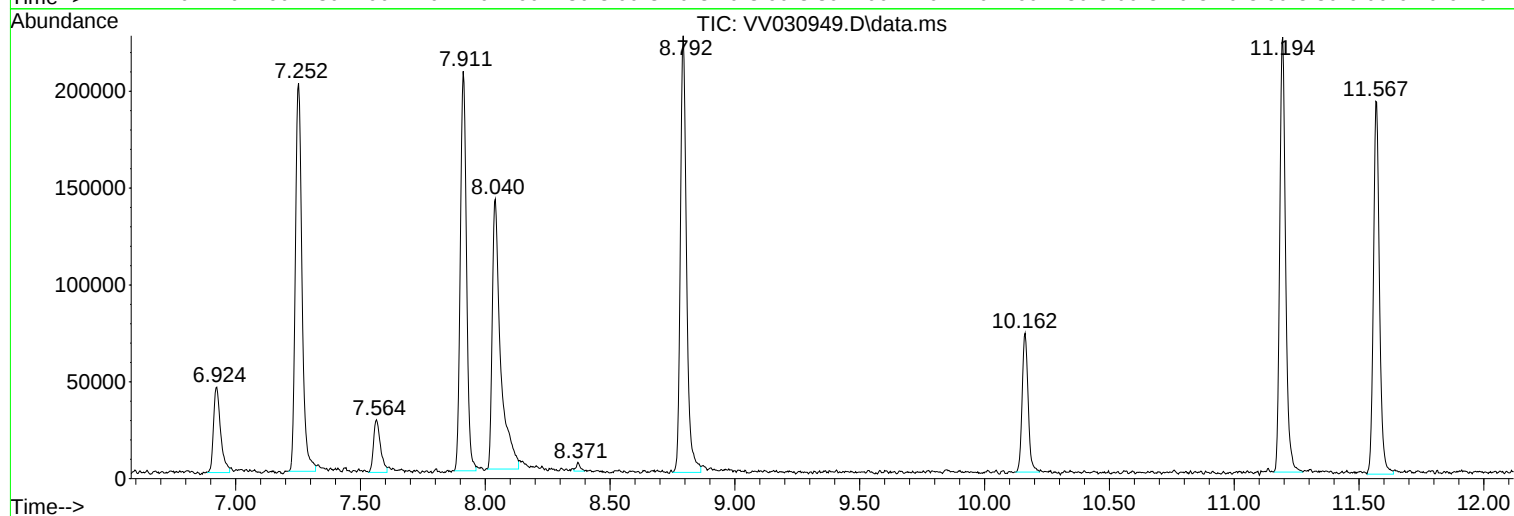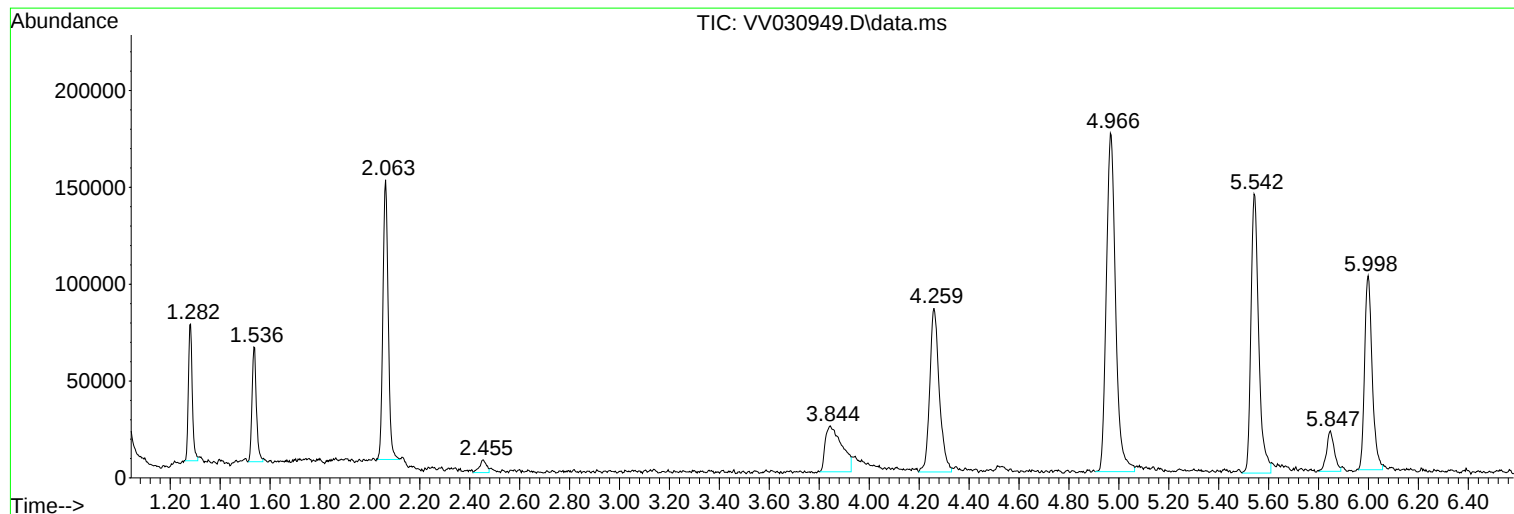

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030949.D
Acq On : 01 May 2023 12:37
Operator : SY/MD
Sample : 02528-04 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030949.D
Acq On : 01 May 2023 12:37
Operator : SY/MD
Sample : 02528-04 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------