

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
 Data File : VV030950.D
 Acq On : 01 May 2023 13:02
 Operator : SY/MD
 Sample : 02528-05 250X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 HOA37

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rVB	63116	67796	7.95%	1.476%
2	1.535	146	154	164	rBV	56515	68128	7.98%	1.484%
3	2.063	307	318	334	rVB2	150243	234511	27.48%	5.107%
4	2.452	432	439	450	rVB6	5335	8952	1.05%	0.195%
5	3.850	860	874	902	rBV	25761	123749	14.50%	2.695%
6	4.259	987	1001	1022	rBV3	77014	197727	23.17%	4.306%
7	4.966	1206	1221	1244	rBV3	165364	423209	49.60%	9.216%
8	5.542	1386	1400	1419	rBV	144049	309564	36.28%	6.741%
9	5.841	1480	1493	1514	rBV2	45457	101272	11.87%	2.205%
10	5.998	1531	1542	1563	rBV2	96127	205690	24.11%	4.479%
11	6.924	1818	1830	1849	rBV	41259	83939	9.84%	1.828%
12	7.252	1920	1932	1955	rBV	185467	341652	40.04%	7.440%
13	7.564	2017	2029	2043	rBV	26304	49792	5.84%	1.084%
14	7.911	2121	2137	2154	rBV	500103	853257	100.00%	18.581%
15	8.040	2165	2177	2202	rBV	144619	333261	39.06%	7.257%
16	8.792	2399	2411	2431	rBV	231504	393656	46.14%	8.573%
17	10.162	2826	2837	2854	rVB3	73948	125286	14.68%	2.728%
18	11.194	3147	3158	3175	rBV	228739	366747	42.98%	7.987%
19	11.570	3262	3275	3290	rBV	185083	303794	35.60%	6.616%




Sum of corrected areas: 4591982

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030950.D
Acq On : 01 May 2023 13:02
Operator : SY/MD
Sample : 02528-05 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

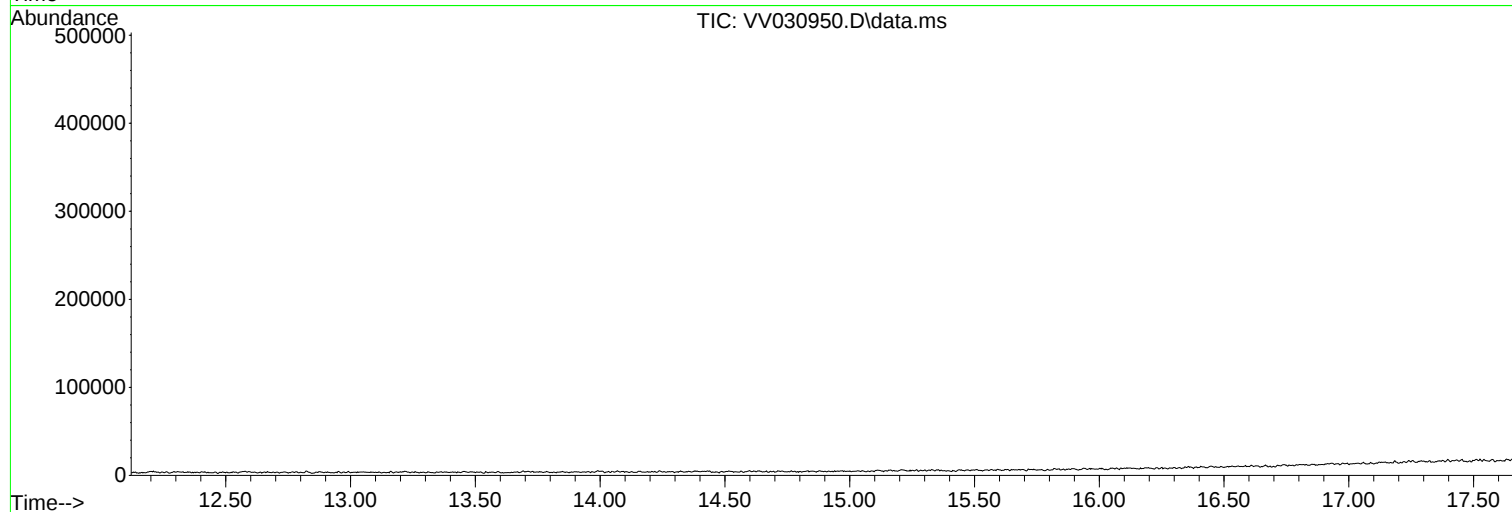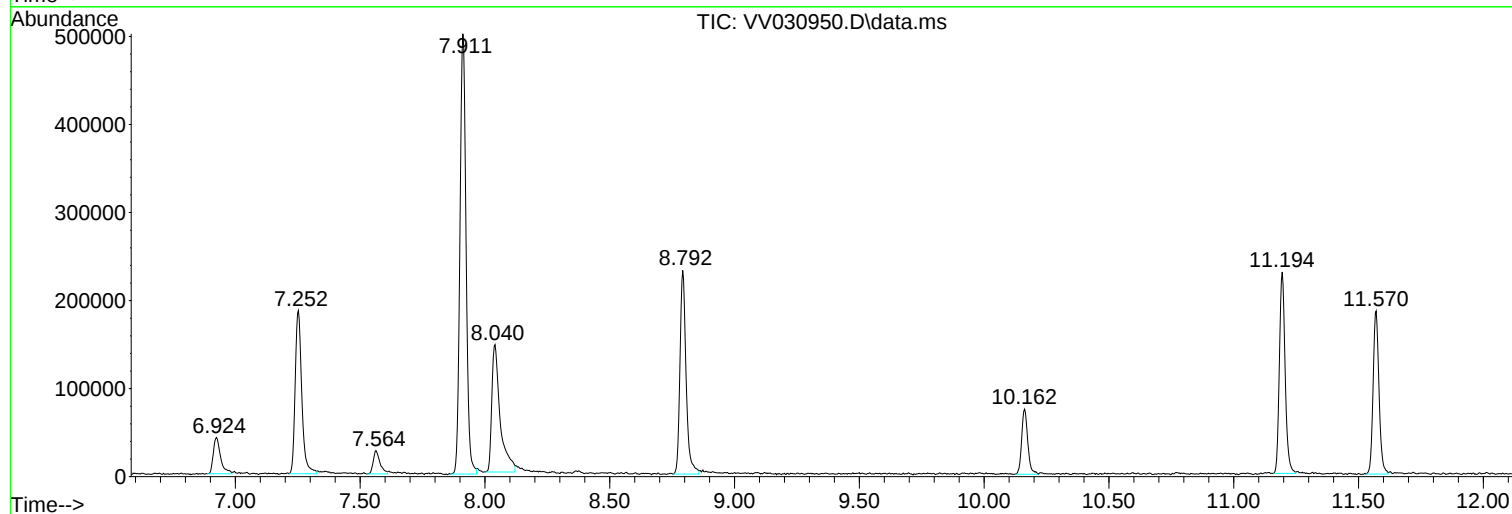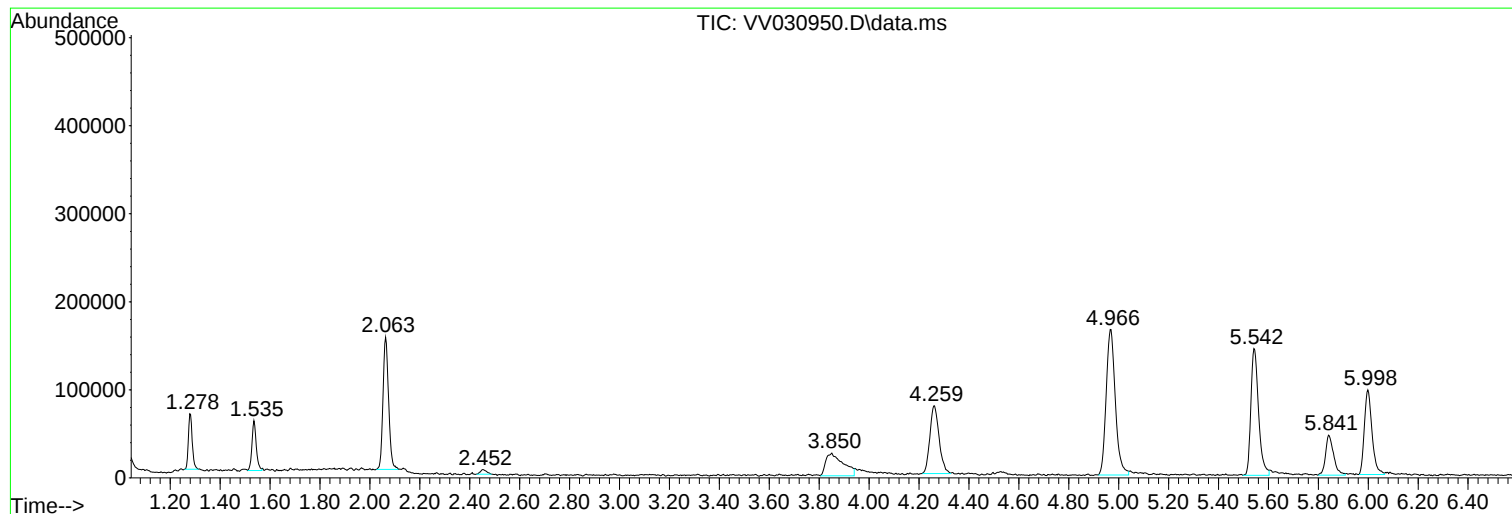

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030950.D
Acq On : 01 May 2023 13:02
Operator : SY/MD
Sample : 02528-05 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030950.D
Acq On : 01 May 2023 13:02
Operator : SY/MD
Sample : 02528-05 250X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc