

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
 Data File : VV030953.D
 Acq On : 01 May 2023 14:16
 Operator : SY/MD
 Sample : 02488-11DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE66DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	88	rVB	76704	79445	15.13%	1.515%
2	1.536	147	154	170	rVB	59981	75876	14.45%	1.447%
3	2.066	307	319	347	rVB3	190516	327315	62.33%	6.243%
4	2.455	428	440	450	rBV	24557	44408	8.46%	0.847%
5	3.835	856	869	905	rBV4	39812	175111	33.34%	3.340%
6	4.262	984	1002	1029	rBV	90250	260210	49.55%	4.963%
7	4.526	1075	1084	1098	rVB10	6287	15168	2.89%	0.289%
8	4.966	1202	1221	1247	rBV2	182016	472352	89.94%	9.009%
9	5.542	1384	1400	1423	rBV	196960	428597	81.61%	8.175%
10	5.841	1477	1493	1517	rBV2	231476	478521	91.12%	9.127%
11	5.998	1528	1542	1562	rBV2	108317	225064	42.86%	4.293%
12	6.921	1818	1829	1853	rBV2	45814	97196	18.51%	1.854%
13	7.252	1917	1932	1954	rBV	203526	382649	72.86%	7.299%
14	7.564	2020	2029	2039	rBV2	28896	51162	9.74%	0.976%
15	7.912	2120	2137	2153	rBV3	140590	253151	48.20%	4.829%
16	8.037	2167	2176	2209	rBV	146901	351448	66.92%	6.703%
17	8.793	2399	2411	2432	rBV	309977	525168	100.00%	10.017%
18	10.162	2825	2837	2848	rBV2	75730	127001	24.18%	2.422%
19	10.333	2879	2890	2900	rBV2	19237	31498	6.00%	0.601%
20	11.194	3144	3158	3177	rBV	311263	501363	95.47%	9.563%
21	11.567	3263	3274	3296	rVB	201123	331612	63.14%	6.325%
22	12.204	3462	3472	3478	rBV10	6338	8520	1.62%	0.163%




Sum of corrected areas: 5242835

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030953.D
Acq On : 01 May 2023 14:16
Operator : SY/MD
Sample : 02488-11DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE66DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

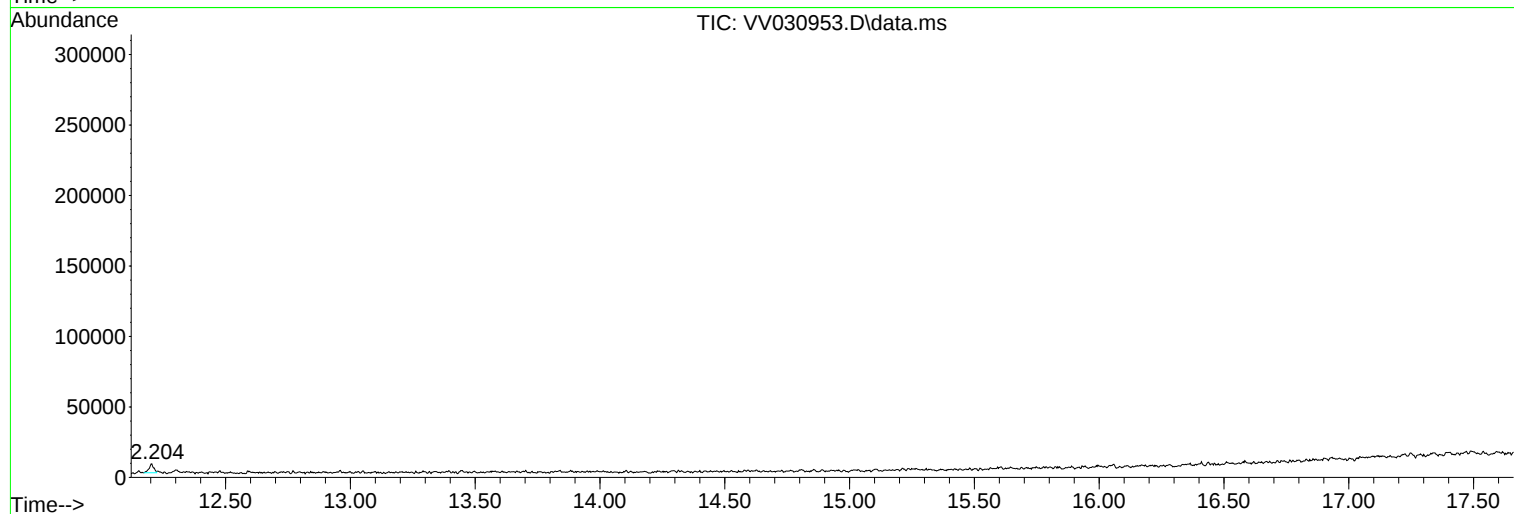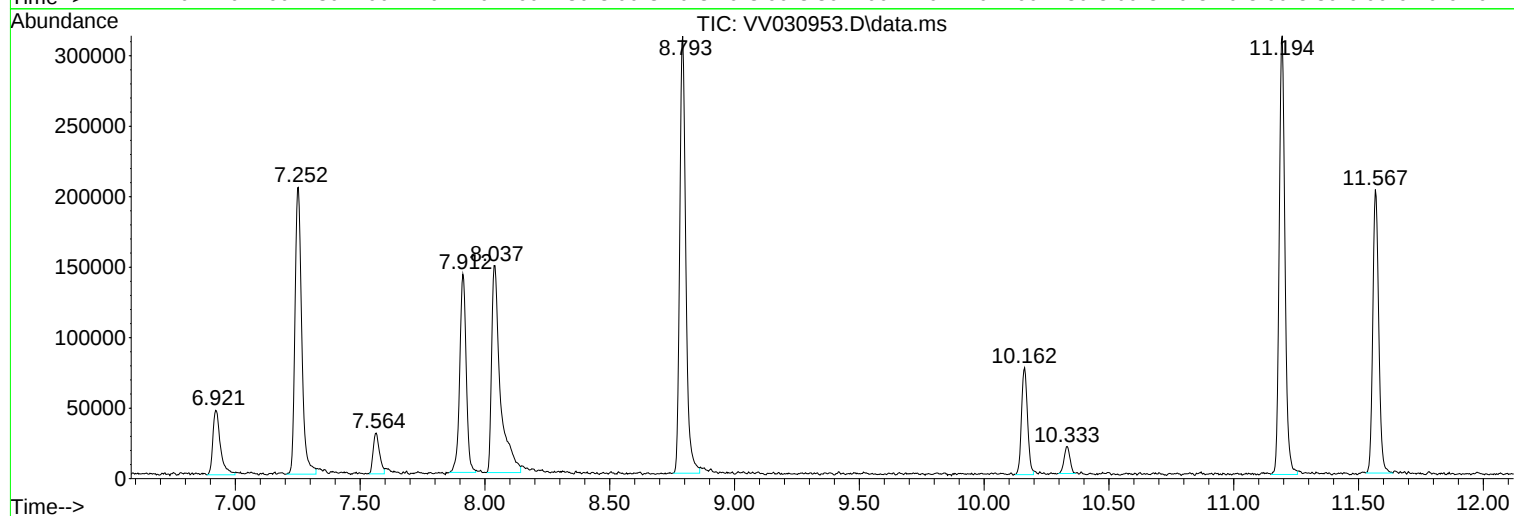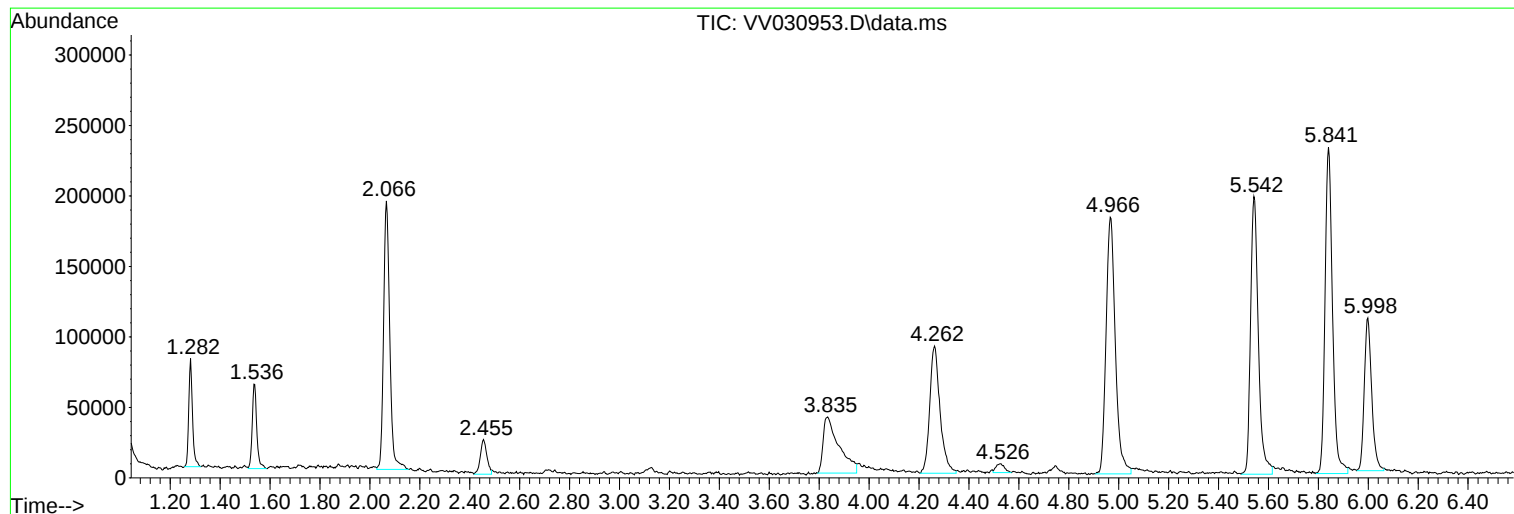

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030953.D
Acq On : 01 May 2023 14:16
Operator : SY/MD
Sample : 02488-11DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE66DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030953.D
Acq On : 01 May 2023 14:16
Operator : SY/MD
Sample : 02488-11DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE66DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc