

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
 Data File : VV030954.D
 Acq On : 01 May 2023 14:40
 Operator : SY/MD
 Sample : 02528-09 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 HOA39

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	86	rBV	64744	72498	16.62%	1.766%
2	1.539	147	155	165	rVV	57140	67846	15.55%	1.653%
3	2.063	309	318	336	rVB	134925	199927	45.82%	4.870%
4	2.452	431	439	441	rBV7	6855	7608	1.74%	0.185%
5	3.828	852	867	892	rBV2	34841	135165	30.98%	3.293%
6	4.259	987	1001	1022	rBV	78064	203423	46.62%	4.955%
7	4.966	1203	1221	1243	rBV3	164584	436309	100.00%	10.628%
8	5.542	1388	1400	1422	rBV	150211	321180	73.61%	7.824%
9	5.844	1483	1494	1508	rBV4	21214	44658	10.24%	1.088%
10	5.998	1528	1542	1561	rBV2	99035	213902	49.03%	5.211%
11	6.921	1814	1829	1846	rBV2	43698	89893	20.60%	2.190%
12	7.252	1916	1932	1955	rBV	187925	352562	80.81%	8.588%
13	7.564	2019	2029	2043	rBV	26400	47439	10.87%	1.156%
14	7.912	2119	2137	2159	rBV	201990	361991	82.97%	8.818%
15	8.037	2165	2176	2203	rBV	142295	311118	71.31%	7.579%
16	8.793	2399	2411	2430	rBV	232267	404697	92.75%	9.858%
17	10.162	2826	2837	2849	rBV	68330	112951	25.89%	2.751%
18	10.336	2883	2891	2898	rVB3	10036	15448	3.54%	0.376%
19	11.194	3146	3158	3176	rBV	234071	388019	88.93%	9.452%
20	11.571	3263	3275	3290	rBV	189049	313642	71.89%	7.640%
21	12.201	3465	3471	3473	rBV6	4705	4913	1.13%	0.120%




Sum of corrected areas: 4105189

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030954.D
Acq On : 01 May 2023 14:40
Operator : SY/MD
Sample : 02528-09 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

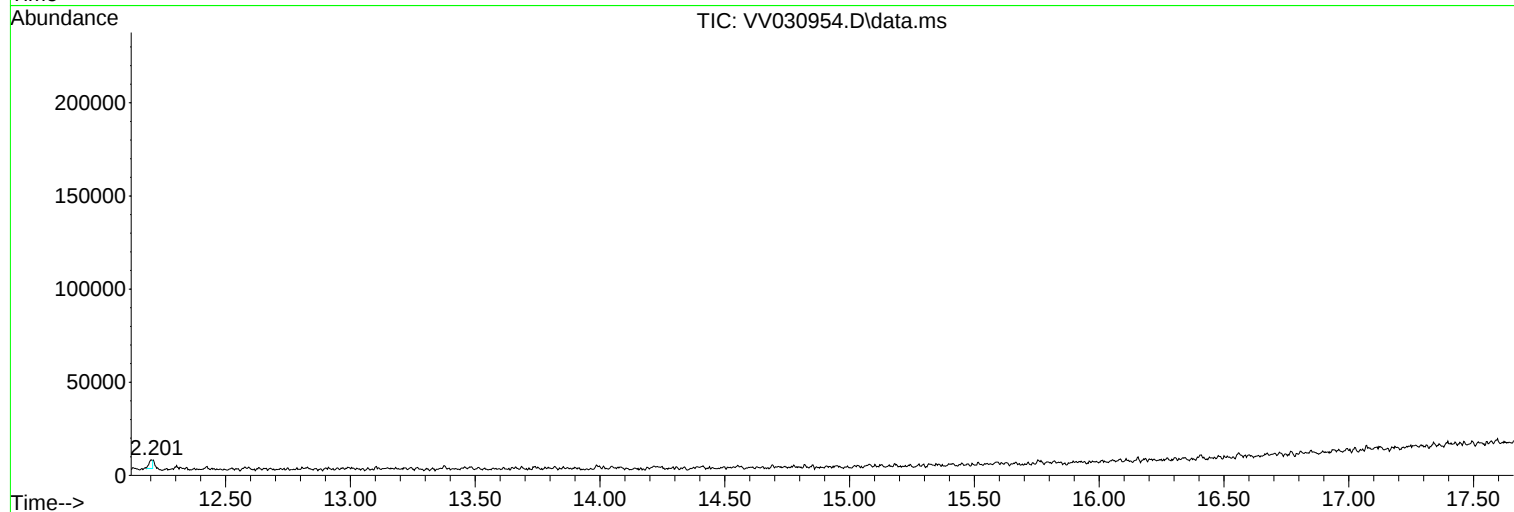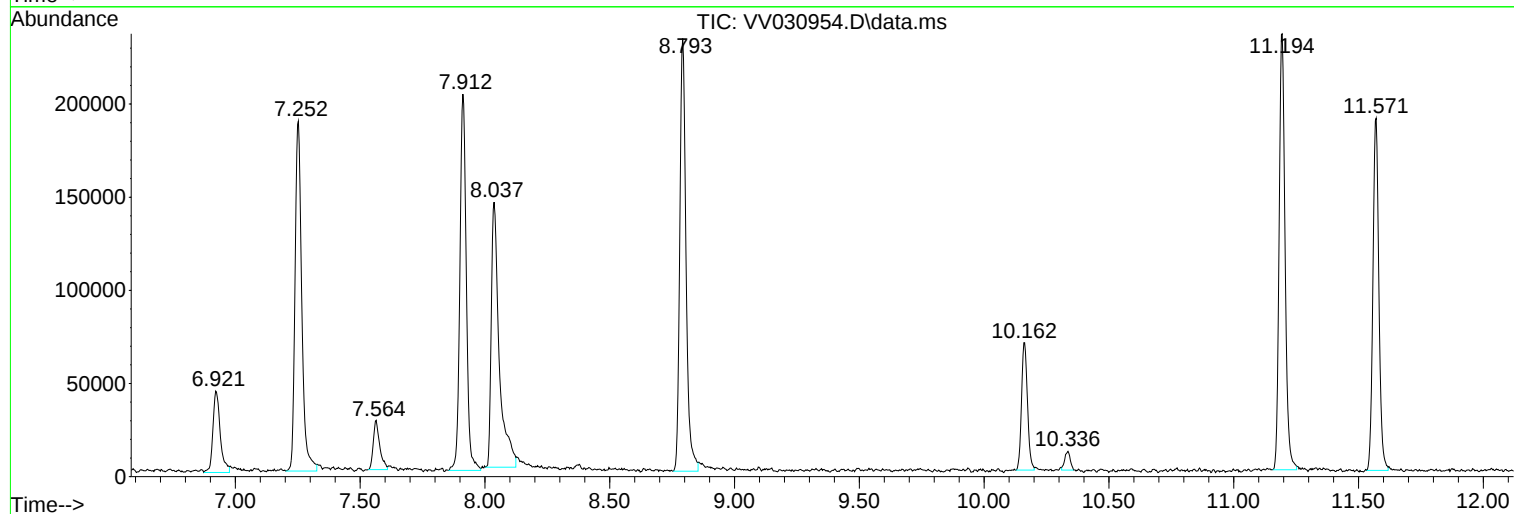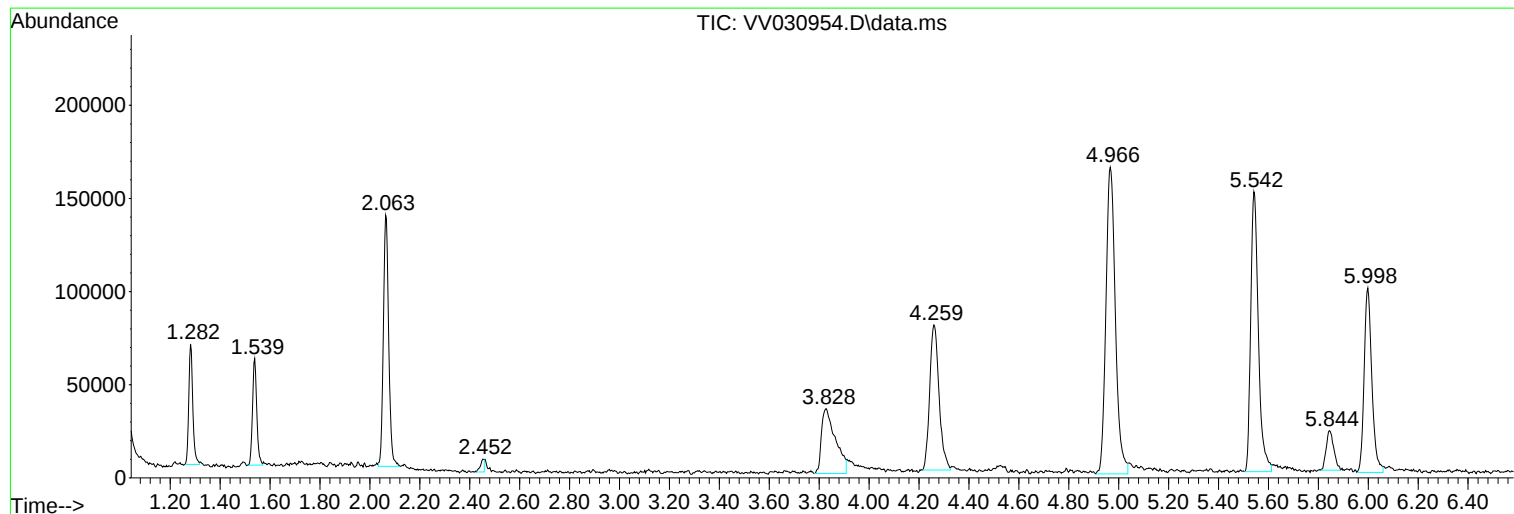

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030954.D
Acq On : 01 May 2023 14:40
Operator : SY/MD
Sample : 02528-09 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030954.D
Acq On : 01 May 2023 14:40
Operator : SY/MD
Sample : 02528-09 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
HOA39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc