

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
 Data File : VV030958.D
 Acq On : 01 May 2023 16:13
 Operator : SY/MD
 Sample : 02551-04DL 500X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHE80DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030958.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	64	75	89	rBV	66940	76284	8.79%	1.635%
2	1.536	147	154	166	rBV	54294	68978	7.95%	1.479%
3	2.063	309	318	333	rVB	134832	194604	22.43%	4.171%
4	2.455	431	440	454	rBV2	21255	37616	4.34%	0.806%
5	3.834	857	869	892	rBV3	36686	138597	15.98%	2.971%
6	4.262	986	1002	1003	rBV2	78888	117132	13.50%	2.511%
7	4.966	1204	1221	1247	rBV2	169953	442031	50.96%	9.475%
8	5.545	1387	1401	1419	rBV	152273	326930	37.69%	7.008%
9	5.847	1483	1495	1507	rBV3	21617	45176	5.21%	0.968%
10	5.998	1529	1542	1562	rBV2	99884	214974	24.78%	4.608%
11	6.924	1819	1830	1846	rBV	43387	83707	9.65%	1.794%
12	7.252	1918	1932	1948	rBV	189867	344601	39.73%	7.387%
13	7.564	2016	2029	2045	rBV2	28290	57576	6.64%	1.234%
14	7.911	2117	2137	2159	rBV	496436	867414	100.00%	18.593%
15	8.037	2166	2176	2204	rBV	165524	366185	42.22%	7.849%
16	8.792	2399	2411	2429	rBV	239016	405643	46.76%	8.695%
17	10.162	2825	2837	2854	rVB	77184	130245	15.02%	2.792%
18	10.333	2878	2890	2902	rBV2	17243	31246	3.60%	0.670%
19	11.194	3145	3158	3177	rBV	242004	389928	44.95%	8.358%
20	11.571	3262	3275	3292	rBV	192248	313841	36.18%	6.727%
21	12.204	3461	3472	3480	rBV5	7616	12532	1.44%	0.269%




Sum of corrected areas: 4665240

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030958.D
Acq On : 01 May 2023 16:13
Operator : SY/MD
Sample : 02551-04DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

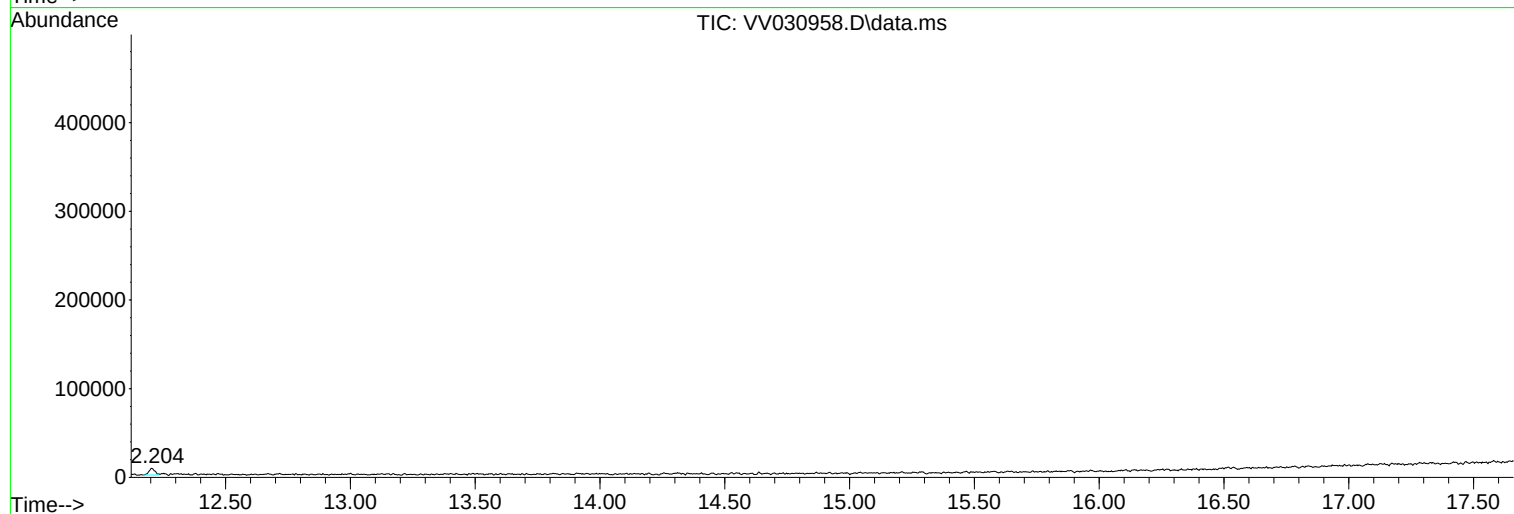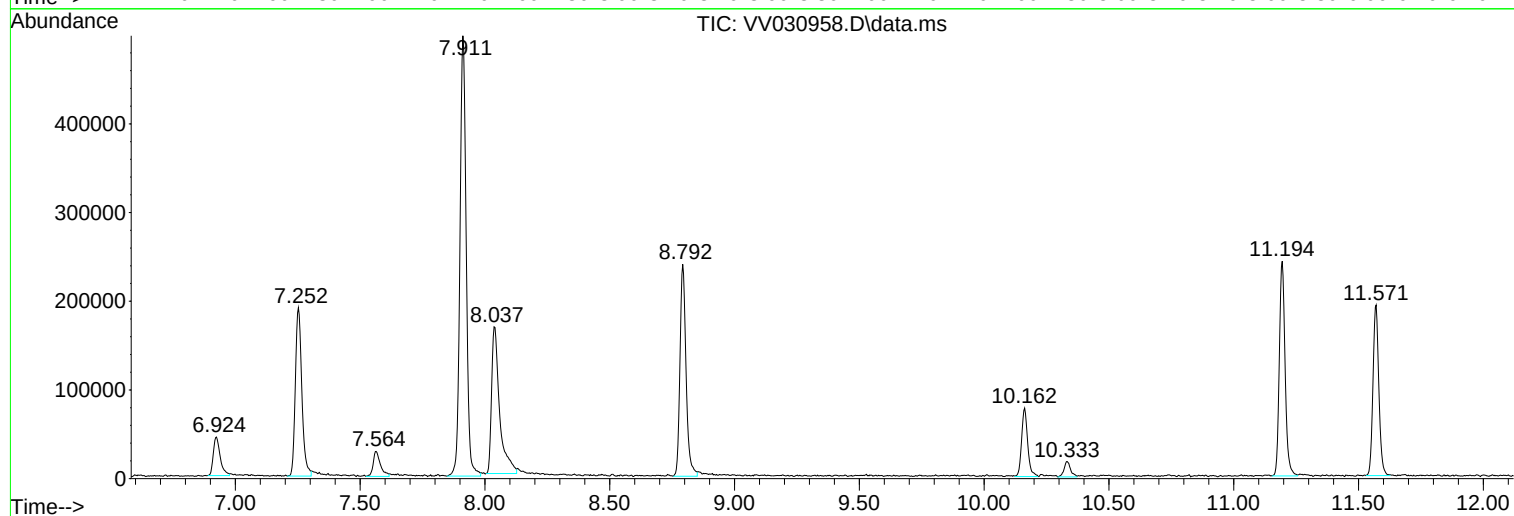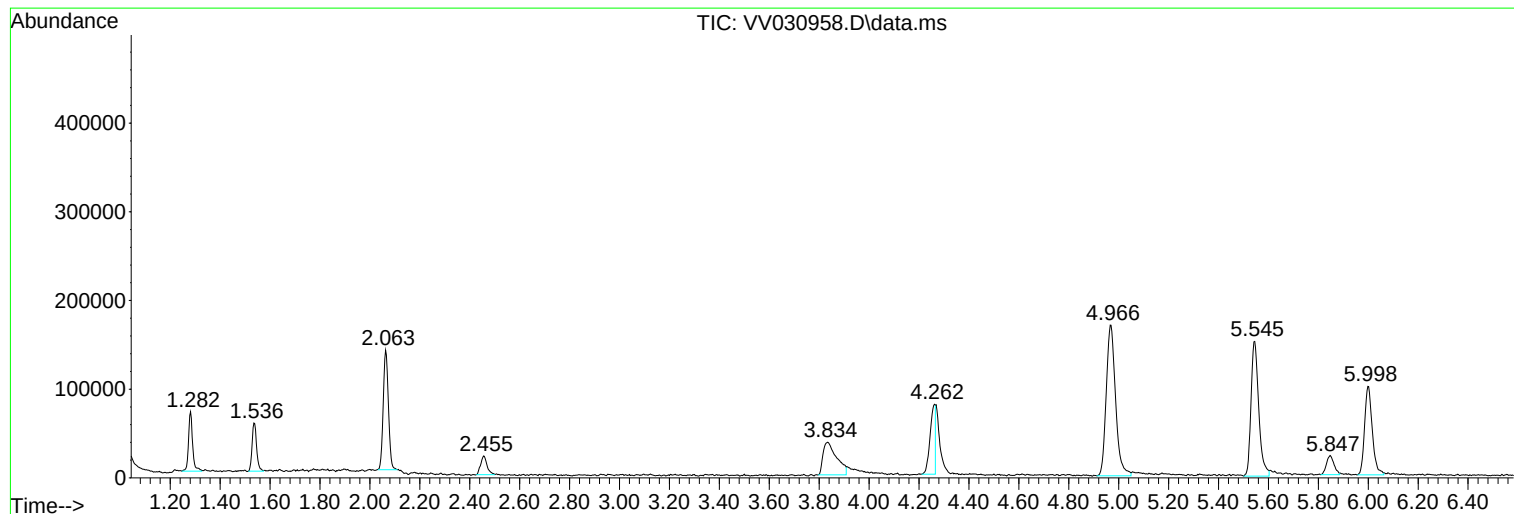

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030958.D
Acq On : 01 May 2023 16:13
Operator : SY/MD
Sample : 02551-04DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030958.D
Acq On : 01 May 2023 16:13
Operator : SY/MD
Sample : 02551-04DL 500X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHE80DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc