

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV050123\  
 Data File : VV030960.D  
 Acq On : 01 May 2023 17:02  
 Operator : SY/MD  
 Sample : 02528-10DL 400X  
 Misc : 25.0mL/MSVOA\_V/WATER  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 HOA40DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR042823WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030960.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.282       | 69            | 75          | 86           | rVB      | 62122          | 65598         | 12.24%          | 1.541%        |
| 2         | 1.536       | 147           | 154         | 168          | rVB      | 53791          | 71061         | 13.26%          | 1.670%        |
| 3         | 2.063       | 310           | 318         | 334          | rVB2     | 140905         | 217620        | 40.60%          | 5.113%        |
| 4         | 2.458       | 430           | 441         | 450          | rBV4     | 8945           | 15434         | 2.88%           | 0.363%        |
| 5         | 3.835       | 857           | 869         | 891          | rBV2     | 29800          | 121007        | 22.57%          | 2.843%        |
| 6         | 4.262       | 986           | 1002        | 1021         | rBV      | 78957          | 205990        | 38.43%          | 4.840%        |
| 7         | 4.966       | 1205          | 1221        | 1245         | rBV2     | 169125         | 432699        | 80.72%          | 10.166%       |
| 8         | 5.545       | 1388          | 1401        | 1424         | rBV      | 136391         | 295447        | 55.12%          | 6.942%        |
| 9         | 5.847       | 1481          | 1495        | 1507         | rBV5     | 28882          | 64959         | 12.12%          | 1.526%        |
| 10        | 5.998       | 1529          | 1542        | 1558         | rBV3     | 99881          | 210027        | 39.18%          | 4.935%        |
| 11        | 6.921       | 1817          | 1829        | 1851         | rBV      | 44211          | 92814         | 17.31%          | 2.181%        |
| 12        | 7.252       | 1920          | 1932        | 1950         | rBV      | 189377         | 343066        | 64.00%          | 8.060%        |
| 13        | 7.561       | 2021          | 2028        | 2046         | rBV2     | 25844          | 48408         | 9.03%           | 1.137%        |
| 14        | 7.912       | 2124          | 2137        | 2154         | rBV      | 311740         | 536033        | 100.00%         | 12.594%       |
| 15        | 8.037       | 2166          | 2176        | 2207         | rBV      | 163442         | 370278        | 69.08%          | 8.700%        |
| 16        | 8.793       | 2398          | 2411        | 2437         | rBV      | 212766         | 371208        | 69.25%          | 8.722%        |
| 17        | 10.162      | 2826          | 2837        | 2857         | rBV2     | 76574          | 128719        | 24.01%          | 3.024%        |
| 18        | 11.194      | 3147          | 3158        | 3174         | rBV      | 224000         | 357524        | 66.70%          | 8.400%        |
| 19        | 11.571      | 3264          | 3275        | 3288         | rBV      | 187737         | 308265        | 57.51%          | 7.243%        |




Sum of corrected areas: 4256157

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV050123\  
Data File : VV030960.D  
Acq On : 01 May 2023 17:02  
Operator : SY/MD  
Sample : 02528-10DL 400X  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
HOA40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR042823WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

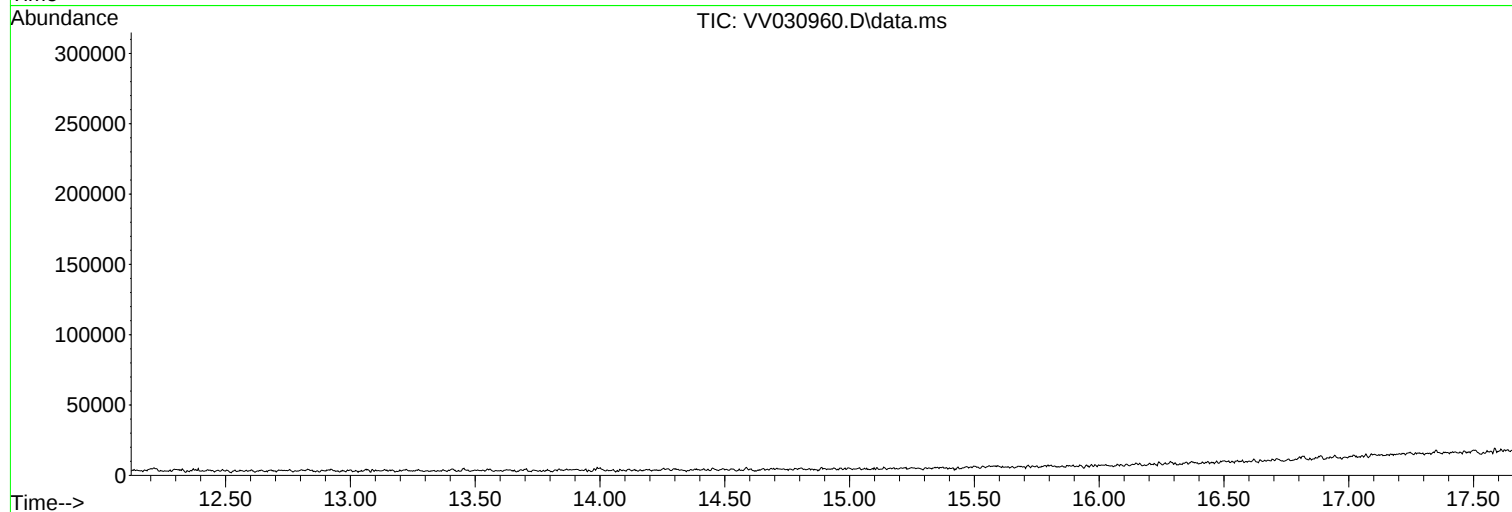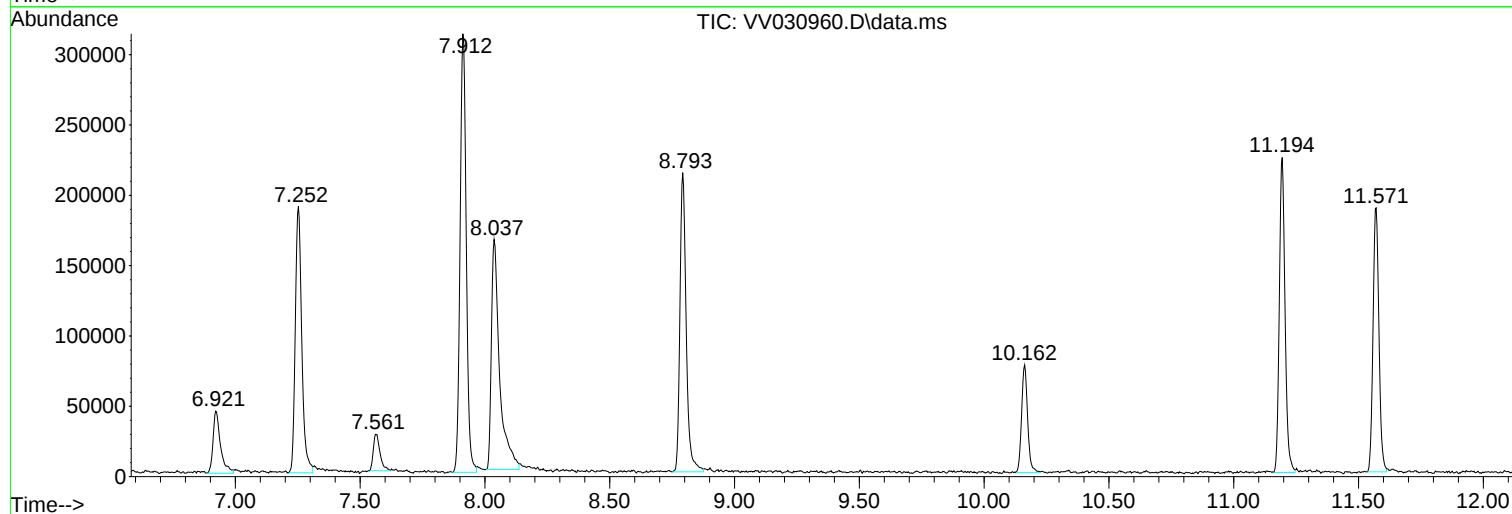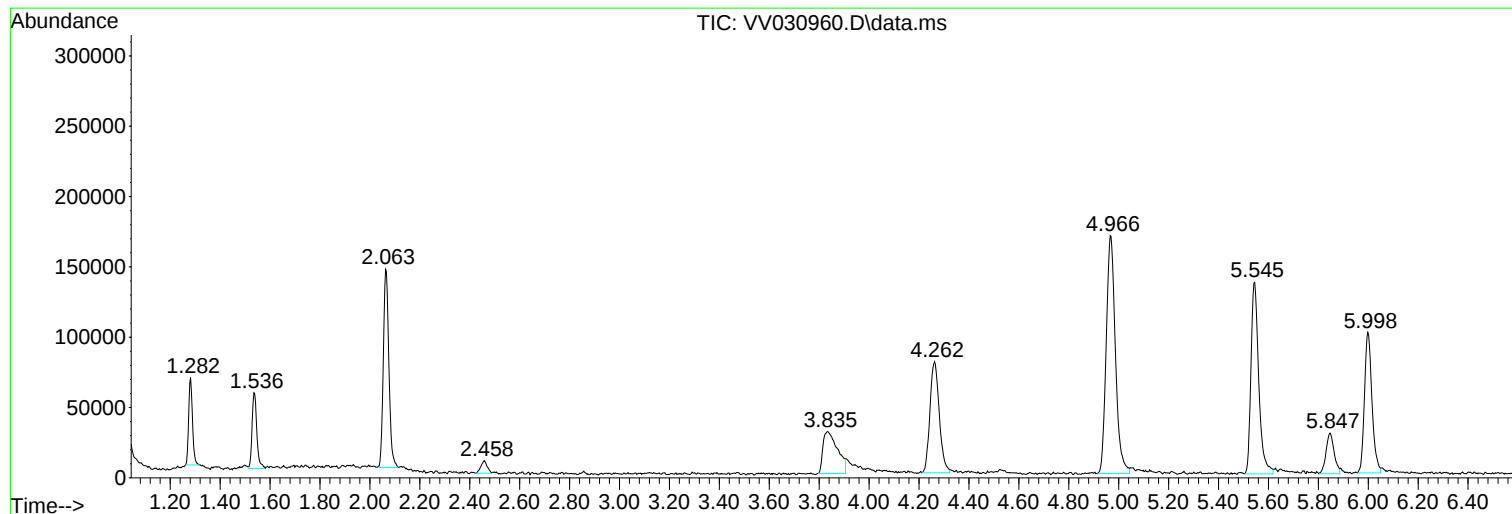

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV050123\  
Data File : VV030960.D  
Acq On : 01 May 2023 17:02  
Operator : SY/MD  
Sample : 02528-10DL 400X  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
HOA40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR042823WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV050123\  
Data File : VV030960.D  
Acq On : 01 May 2023 17:02  
Operator : SY/MD  
Sample : 02528-10DL 400X  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
HOA40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR042823WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |