

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
 Data File : VV030964.D
 Acq On : 01 May 2023 18:41
 Operator : SY/MD
 Sample : VIBLK293
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK293

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	87	rBV	77050	81657	16.62%	1.986%
2	1.535	147	154	166	rVB	60282	74734	15.21%	1.817%
3	2.063	308	318	336	rVB	152011	219314	44.64%	5.333%
4	2.455	432	440	456	rVB5	6561	12058	2.45%	0.293%
5	3.838	858	870	889	rBV	28701	111762	22.75%	2.718%
6	4.262	987	1002	1021	rBV	87563	223203	45.43%	5.428%
7	4.966	1205	1221	1246	rBV2	191890	491295	100.00%	11.947%
8	5.542	1387	1400	1423	rBV	164827	350084	71.26%	8.513%
9	5.998	1528	1542	1559	rBV	111149	241014	49.06%	5.861%
10	6.921	1819	1829	1848	rBV2	47940	96067	19.55%	2.336%
11	7.252	1918	1932	1954	rBV	214232	396891	80.78%	9.652%
12	7.564	2021	2029	2043	rBV	29027	55077	11.21%	1.339%
13	8.037	2165	2176	2208	rBV	158149	380706	77.49%	9.258%
14	8.792	2400	2411	2433	rBV	250133	425722	86.65%	10.353%
15	10.162	2825	2837	2851	rBV2	80005	131216	26.71%	3.191%
16	11.194	3146	3158	3176	rBV	253713	412480	83.96%	10.031%
17	11.570	3263	3275	3290	rBV	214673	349612	71.16%	8.502%
18	12.596	3584	3594	3600	rBV	5598	9023	1.84%	0.219%
19	13.213	3777	3786	3794	rBV7	8834	15836	3.22%	0.385%
20	13.451	3851	3860	3869	rBV3	11239	18710	3.81%	0.455%
21	13.689	3925	3934	3946	rVB6	9833	15726	3.20%	0.382%




Sum of corrected areas: 4112187

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030964.D
Acq On : 01 May 2023 18:41
Operator : SY/MD
Sample : VIBLK293
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK293

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

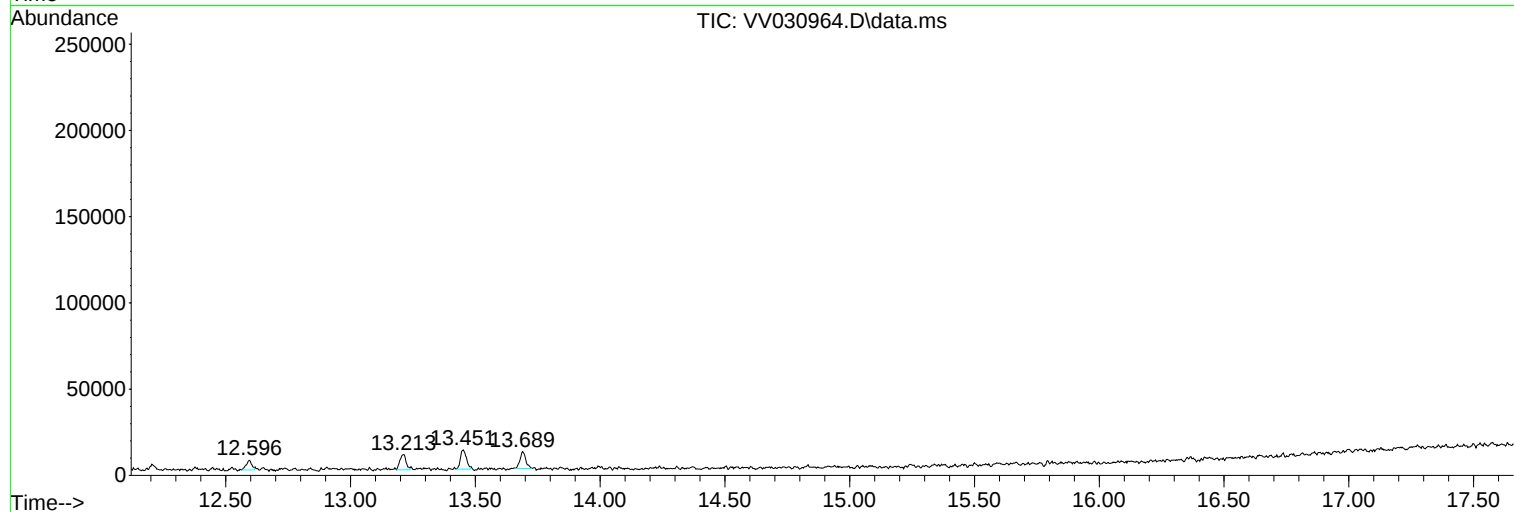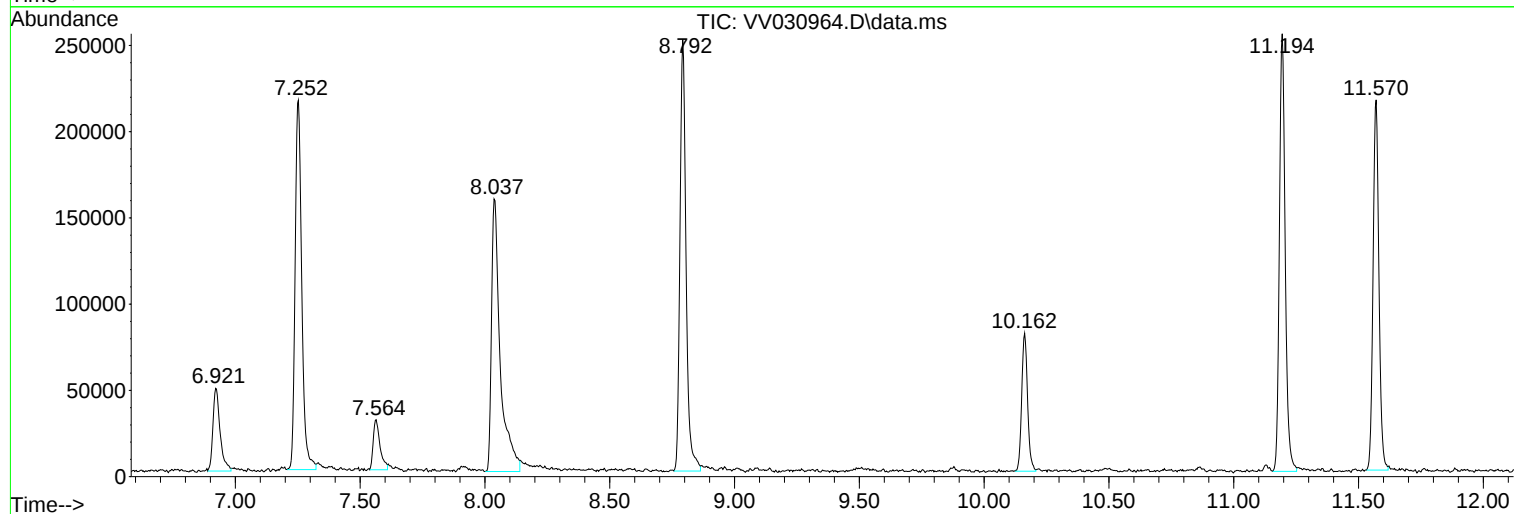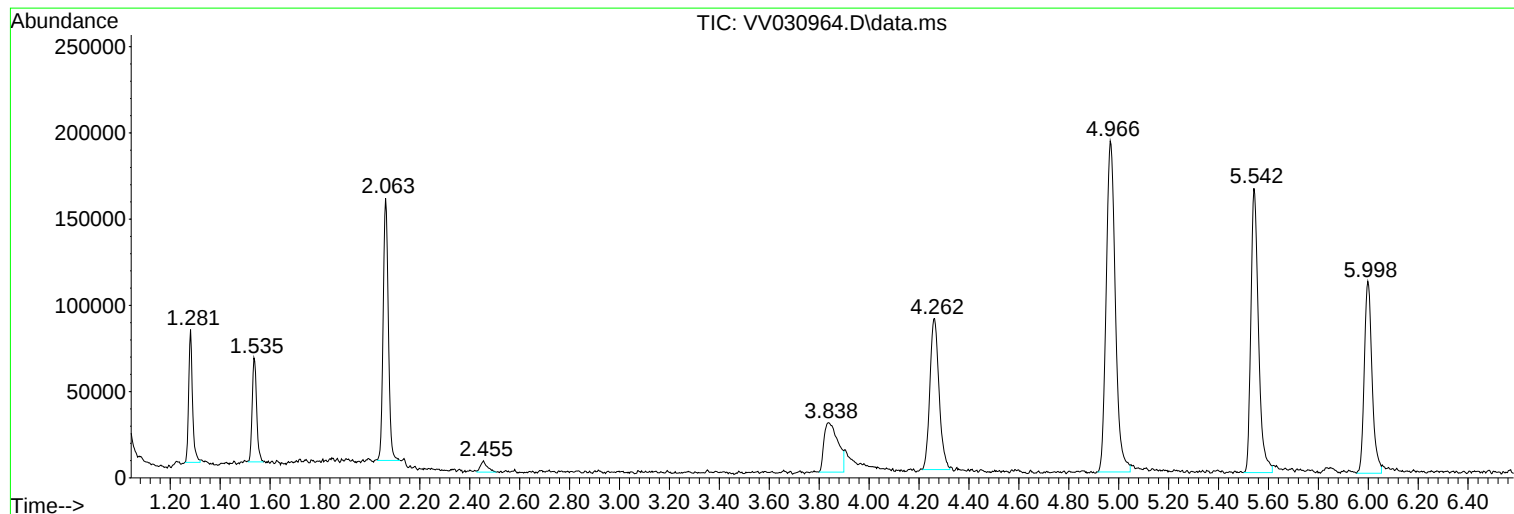

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030964.D
Acq On : 01 May 2023 18:41
Operator : SY/MD
Sample : VIBLK293
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK293

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030964.D
Acq On : 01 May 2023 18:41
Operator : SY/MD
Sample : VIBLK293
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK293

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc