
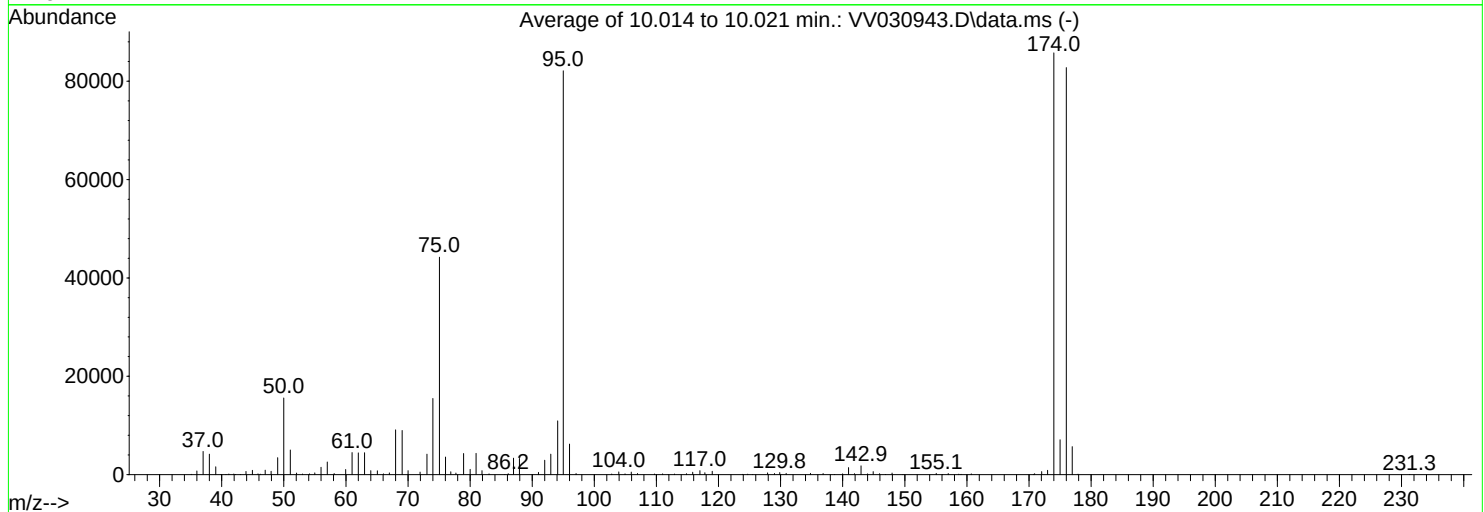


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050123\
Data File : VV030943.D
Acq On : 01 May 2023 09:10
Operator : SY/MD
Sample : BFB256
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB256

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR042823WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Apr 29 01:06:38 2023

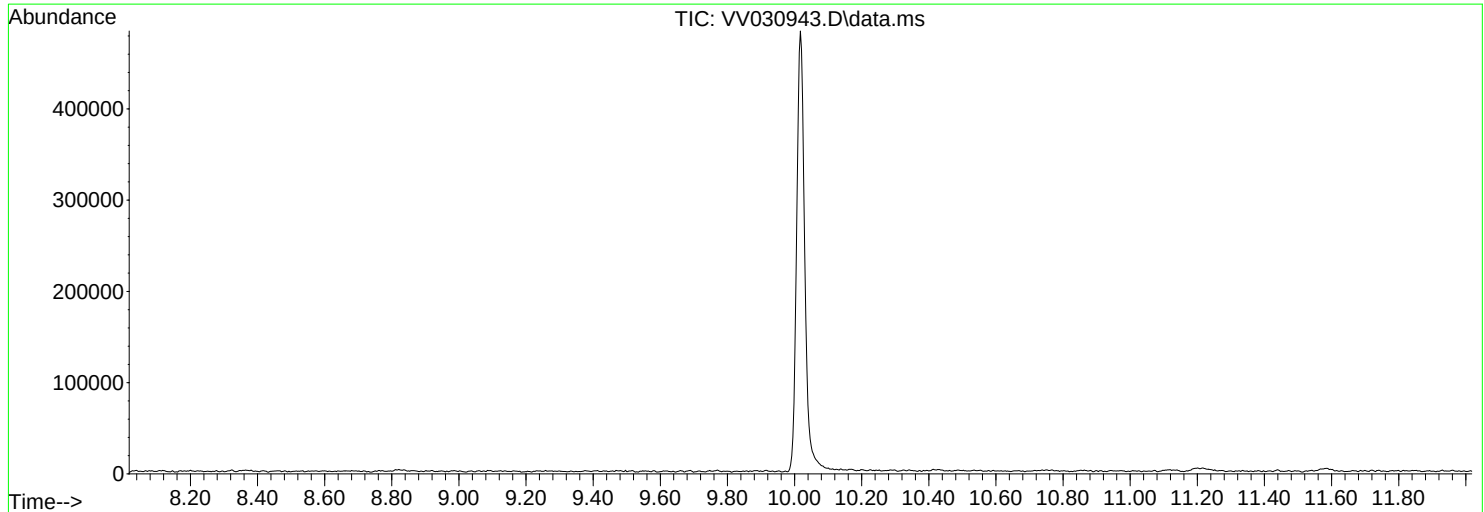

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	15596	PASS
75	95	30	80	53.8	44213	PASS
95	95	100	100	100.0	82117	PASS
96	95	5	9	7.6	6202	PASS
173	174	0.00	2	1.0	868	PASS
174	95	50	120	104.5	85776	PASS
175	174	5	9	8.3	7103	PASS
176	174	95	105	96.5	82773	PASS
177	176	5	10	6.9	5688	PASS

m/z	Abundance
35.50	110.0
36.00	133.0
36.90	105.0
37.90	141.0
38.60	120.0
38.80	121.0
39.90	224.0
41.50	105.0
42.60	103.0
43.10	160.0
43.90	168.0
44.90	110.0
47.70	123.0
48.40	140.0
49.70	114.0
51.20	114.0
53.00	120.0
57.70	116.0
58.60	106.0
61.50	102.0
72.00	118.0
72.60	104.0
78.50	115.0
81.40	107.0
93.70	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
36.00	889.0
37.10	4678.0
38.00	4338.0
39.10	1642.0
40.10	227.0
41.10	154.0
42.00	138.0
42.90	200.0
44.00	705.0
45.00	1014.0
45.90	169.0
47.00	878.0
47.90	735.0
49.00	3479.0
50.00	15477.0
51.00	5125.0
52.00	345.0
53.00	201.0
54.10	134.0
55.00	283.0
56.00	1452.0
57.00	2475.0
58.10	210.0
60.00	1000.0
61.00	4371.0
62.00	4219.0
63.00	4585.0
64.00	767.0
65.10	772.0
66.10	184.0
67.00	362.0
68.00	8931.0
69.00	8965.0
70.00	842.0
71.90	659.0
73.10	4148.0
74.00	15114.0
75.10	43712.0
76.00	3608.0
76.90	571.0
77.80	378.0
78.90	4125.0
80.00	1083.0
81.00	4196.0
81.90	811.0
83.10	173.0
86.10	225.0
87.00	3076.0
88.00	3166.0
91.00	460.0
92.00	2997.0
93.00	4020.0
94.10	10532.0
95.00	82024.0
96.00	6041.0
97.00	274.0
102.90	120.0
104.00	529.0
104.90	184.0
106.00	517.0
107.00	219.0
109.70	147.0
111.00	198.0
112.90	143.0
114.80	213.0
115.90	470.0
117.00	776.0
117.80	398.0
119.00	734.0
128.00	384.0
129.10	227.0
129.80	430.0
130.90	213.0
134.80	257.0
136.80	235.0
140.00	138.0
140.90	1395.0
141.90	207.0
143.00	1753.0
144.00	146.0
144.90	510.0
145.90	219.0
148.00	297.0
149.70	112.0
155.10	303.0
157.10	209.0
159.10	108.0
160.80	162.0
170.70	239.0
172.00	562.0
173.00	1283.0
174.00	82856.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

175.00	7078.0
176.00	80872.0
176.90	5535.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
36.00	935.0
37.10	4874.0
38.10	4490.0
39.00	1626.0
39.90	235.0
40.70	116.0
41.20	136.0
42.00	136.0
42.90	213.0
43.90	828.0
45.00	1039.0
45.80	171.0
46.20	158.0
47.00	978.0
47.90	705.0
49.00	3498.0
50.00	16100.0
51.00	5334.0
52.00	346.0
53.10	287.0
54.10	145.0
55.00	381.0
56.00	1557.0
57.00	2668.0
58.10	246.0
59.90	1049.0
61.00	4607.0
62.00	4589.0
63.00	4583.0
64.00	847.0
65.10	848.0
66.00	158.0
67.00	368.0
68.00	9272.0
69.00	9249.0
70.00	899.0
71.90	653.0
73.00	4263.0
74.00	16105.0
75.00	45632.0
76.10	3665.0
76.90	619.0
77.70	358.0
79.00	4376.0
80.00	1121.0
81.00	4443.0
81.90	814.0
83.10	166.0
86.10	216.0
87.00	3475.0
87.90	3407.0
91.00	485.0
92.00	3021.0
93.00	4309.0
94.10	11266.0
95.00	84400.0
96.00	6413.0
97.10	242.0
102.70	111.0
103.90	553.0
105.00	172.0
106.00	541.0
106.90	230.0
109.70	151.0
111.00	184.0
112.90	121.0
114.80	178.0
115.80	487.0
117.00	854.0
117.80	386.0
119.00	736.0
123.90	104.0
124.70	108.0
125.50	101.0
127.90	358.0
129.00	236.0
129.90	448.0
130.90	276.0
134.80	287.0
136.90	244.0
140.00	191.0
140.90	1511.0
141.90	204.0
142.90	1846.0
144.00	180.0
144.90	636.0
145.90	200.0
147.90	340.0
155.10	236.0
156.10	105.0
157.00	216.0
158.70	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

159.00	120.0
160.70	191.0
170.90	297.0
172.10	636.0
173.00	1322.0
174.00	88232.0
175.00	7348.0
176.00	85464.0
177.00	5869.0
177.90	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

m/z	Abundance
35.10	175.0
36.00	840.0
37.00	4879.0
38.10	4137.0
39.00	1560.0
39.90	277.0
41.20	120.0
41.90	144.0
42.20	127.0
43.00	202.0
43.90	879.0
45.00	951.0
45.80	165.0
46.20	163.0
47.00	885.0
48.00	641.0
49.00	3341.0
50.00	15210.0
51.10	4977.0
52.10	290.0
53.10	282.0
54.20	183.0
55.00	383.0
56.00	1449.0
57.00	2616.0
58.10	246.0
59.90	1047.0
61.00	4488.0
62.00	4516.0
63.00	4165.0
64.00	815.0
65.00	757.0
66.00	137.0
67.00	367.0
68.00	9133.0
69.10	8719.0
70.00	750.0
72.00	587.0
73.00	4089.0
74.00	15268.0
75.00	43296.0
76.00	3480.0
76.90	595.0
77.60	294.0
79.00	4367.0
80.00	1061.0
80.90	4310.0
81.90	785.0
83.00	137.0
85.60	111.0
86.20	198.0
87.00	3510.0
87.90	3329.0
91.00	465.0
92.00	2754.0
93.00	4130.0
94.10	11028.0
95.00	79928.0
96.00	6153.0
97.10	209.0
102.80	119.0
103.90	543.0
105.00	172.0
105.90	480.0
106.90	223.0
109.70	139.0
111.00	145.0
111.90	104.0
112.90	119.0
114.90	150.0
115.90	488.0
117.00	806.0
117.80	347.0
119.00	615.0
123.90	126.0
124.70	159.0
127.80	344.0
128.90	198.0
129.90	408.0
130.90	267.0
134.80	273.0
136.90	233.0
138.70	120.0
140.00	186.0
141.00	1399.0
141.90	154.0
142.90	1812.0
144.00	178.0
144.90	667.0
146.00	204.0
146.90	107.0
147.90	314.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256

155.00	214.0
156.90	225.0
158.70	170.0
160.60	180.0
170.90	318.0
172.10	696.0
174.00	86240.0
175.00	6883.0
176.00	81984.0
177.00	5660.0
177.90	177.0
231.30	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB256