




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025762.D
Acq On : 02 May 2022 13:47
Operator : SY/MD
Sample : N2612-17
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/09/2022
Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 03 05:23:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 03 05:22:31 2022
Response via : Initial Calibration

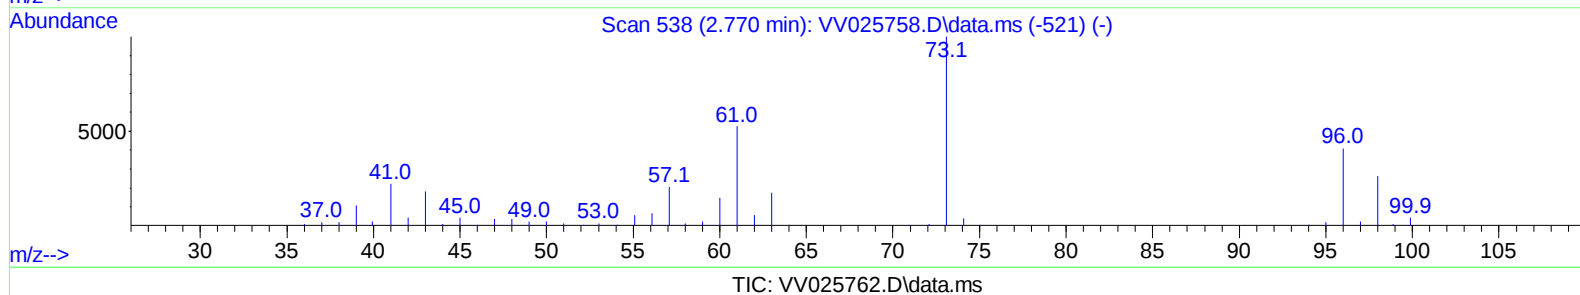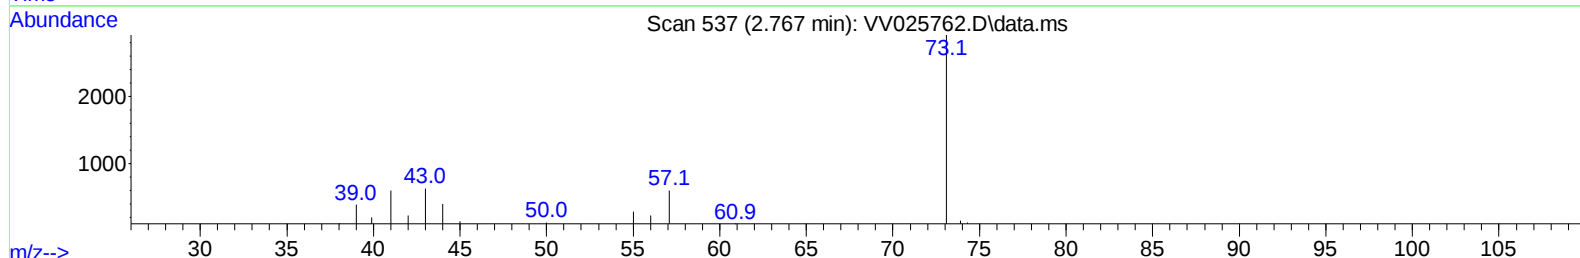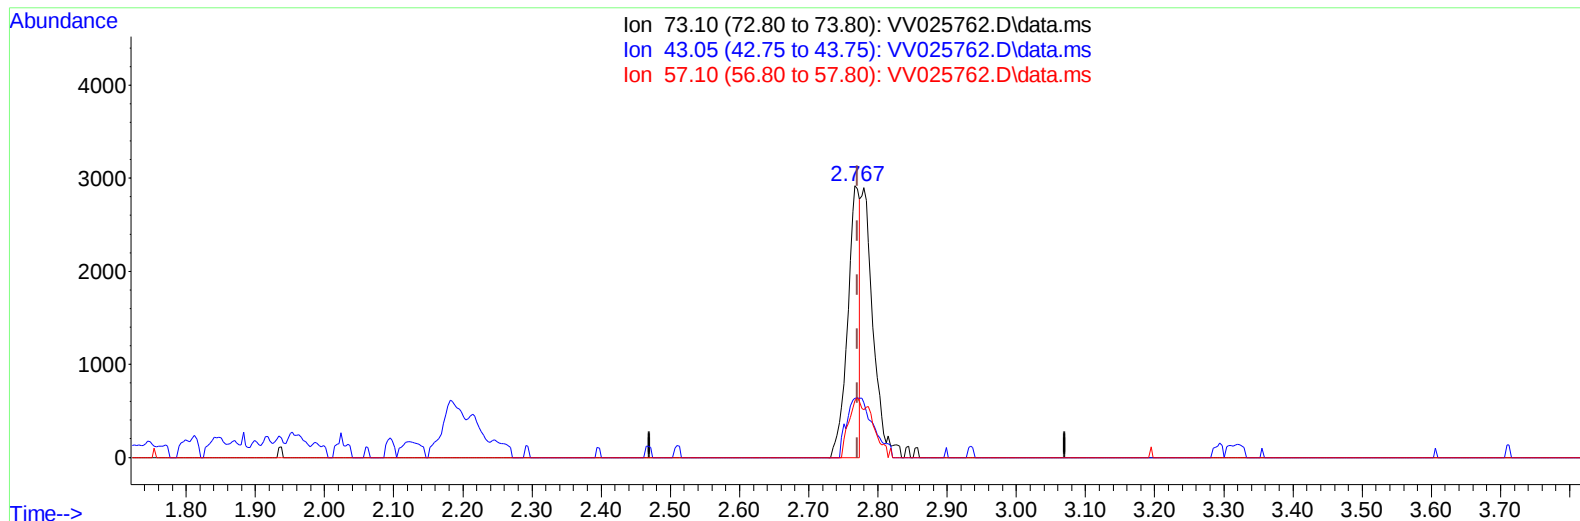

(17) Methyl tert-butyl Ether (T)

2.767min (-0.003) 0.17 ug/L

response 3529

Ion	Exp%	Act%
73.10	100.00	100.00
43.05	17.80	48.06#
57.10	20.10	25.79#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025762.D
 Acq On : 02 May 2022 13:47
 Operator : SY/MD
 Sample : N2612-17
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0C7

Manual IntegrationsAPPROVED

Quant Time: May 03 05:23:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 03 05:22:31 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/09/2022
 Supervised By :Mahesh Dadoda 05/09/2022

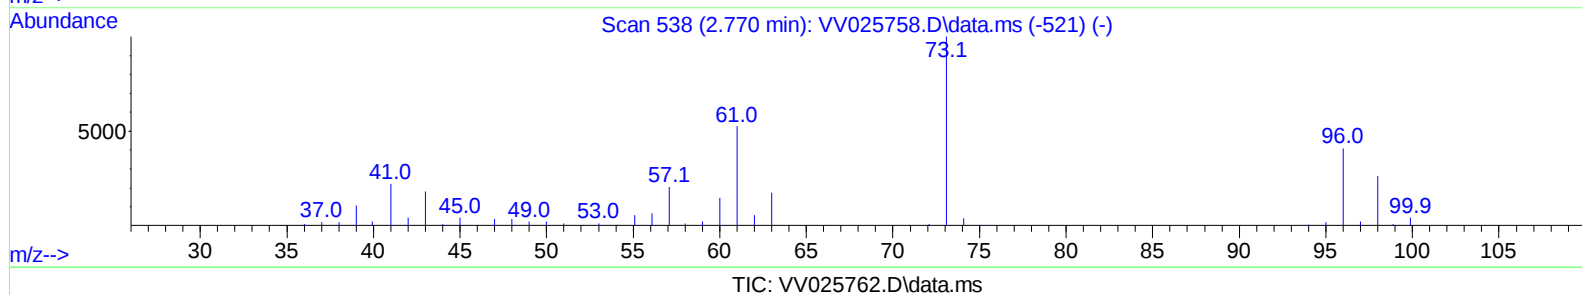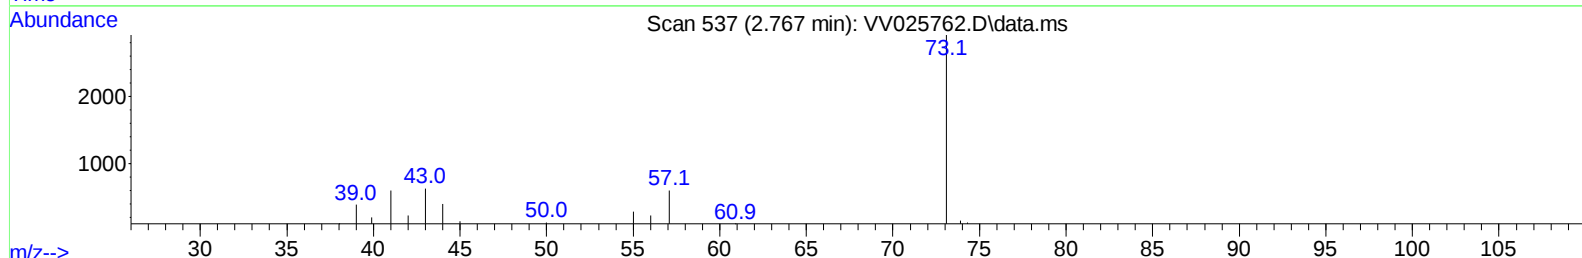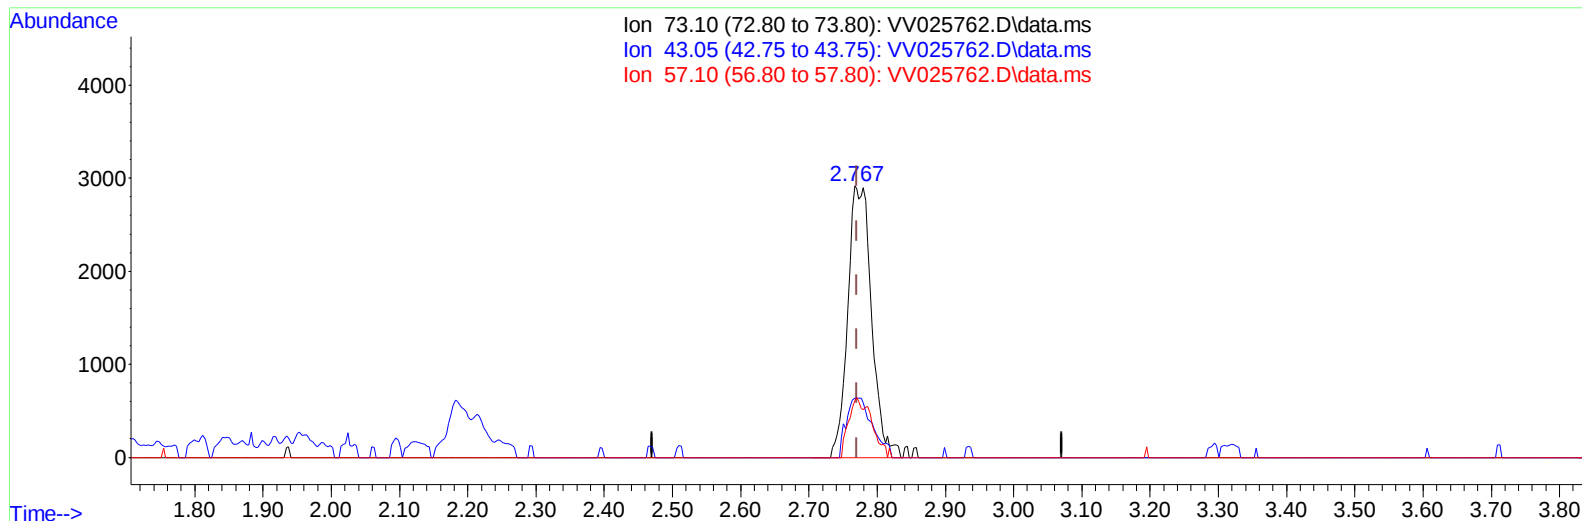

(17) Methyl tert-butyl Ether (T)

2.767min (-0.003) 0.33 ug/L m

response 7057

Ion	Exp%	Act%
73.10	100.00	100.00
43.05	17.80	24.03#
57.10	20.10	12.89#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025762.D
 Acq On : 02 May 2022 13:47
 Operator : SY/MD
 Sample : N2612-17
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0C7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/09/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 03 05:23:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 03 05:22:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	157148	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	162302	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	73428	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	45410	3.108	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	62.200%	
7) Chloroethane-d5	1.571	69	50035	3.219	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	64.400%#	
11) 1,1-Dichloroethene-d2	2.111	63	76198	2.603	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	52.000%#	
20) 2-Butanone-d5	3.899	46	103161	58.047	ug/L	0.01
Spiked Amount 50.000	Range 40	- 130	Recovery	=	116.100%	
24) Chloroform-d	4.352	84	105137	4.762	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	95.200%	
26) 1,2-Dichloroethane-d4	5.037	65	49936	5.249	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	105.000%	
32) Benzene-d6	5.053	84	193330	4.117	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	82.400%	
36) 1,2-Dichloropropane-d6	6.069	67	62762	4.792	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	95.800%	
41) Toluene-d8	7.317	98	154860	3.554	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	71.000%	
43) trans-1,3-Dichloroprop...	7.628	79	13242	3.008	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	60.200%	
46) 2-Hexanone-d5	8.088	63	74826	48.433	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	96.860%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	44185	5.340	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	106.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	57947	4.707	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	94.200%	
Target Compounds						
5) Vinyl chloride	1.314	62	3468	0.199	ug/L #	80
17) Methyl tert-butyl Ether	2.767	73	7057m	0.335	ug/L	
47) Tetrachloroethene	7.982	164	1113	0.112	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025762.D
Acq On : 02 May 2022 13:47
Operator : SY/MD
Sample : N2612-17
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/09/2022
Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 03 05:23:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 03 05:22:31 2022
Response via : Initial Calibration

