




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025765.D
 Acq On : 02 May 2022 14:57
 Operator : SY/MD
 Sample : N2621-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFJ8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/09/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 03 05:24:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 03 05:22:31 2022
 Response via : Initial Calibration

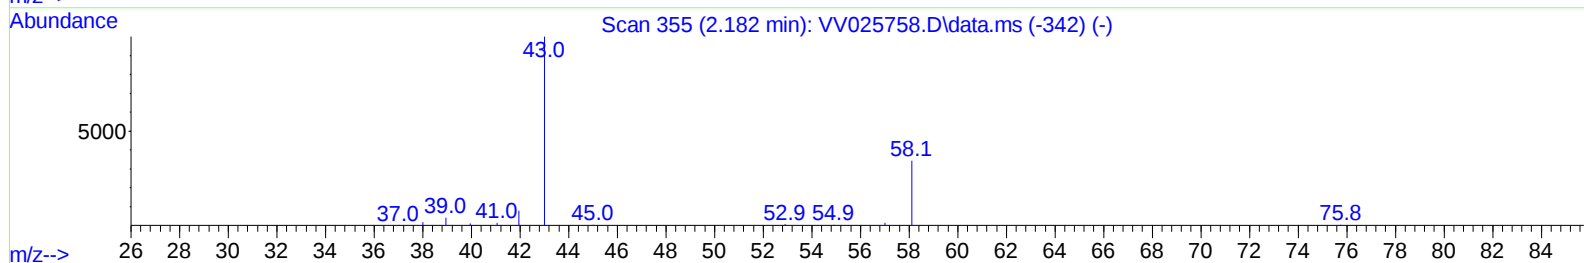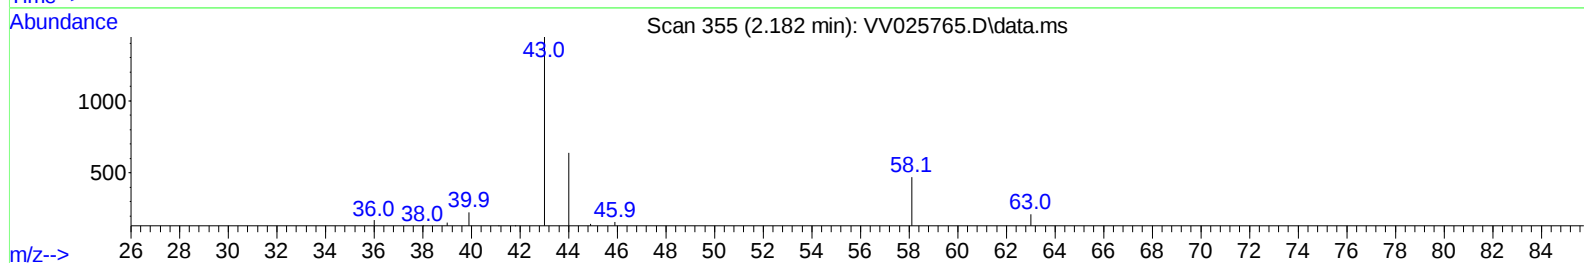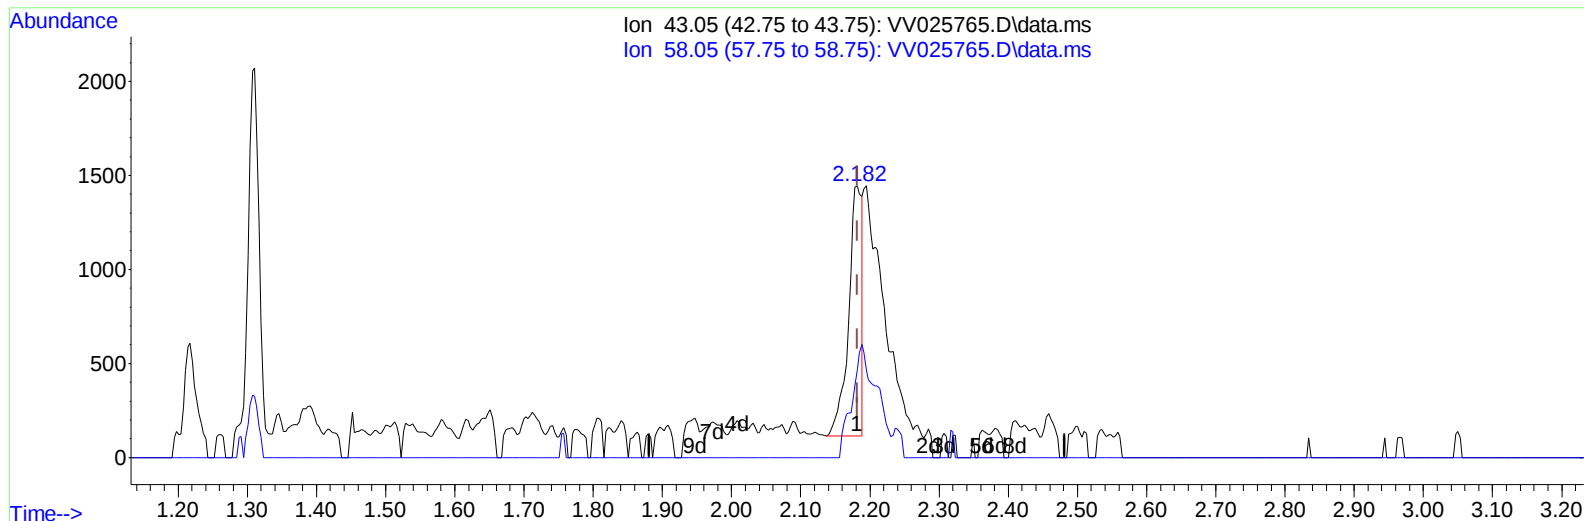

TIC: VV025765.D\data.ms

(13) Acetone (T)

2.182min (-0.000) 1.45 ug/L

response 1789

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	82.62#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025765.D
 Acq On : 02 May 2022 14:57
 Operator : SY/MD
 Sample : N2621-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFJ8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/09/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Quant Time: May 03 05:24:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 03 05:22:31 2022
 Response via : Initial Calibration

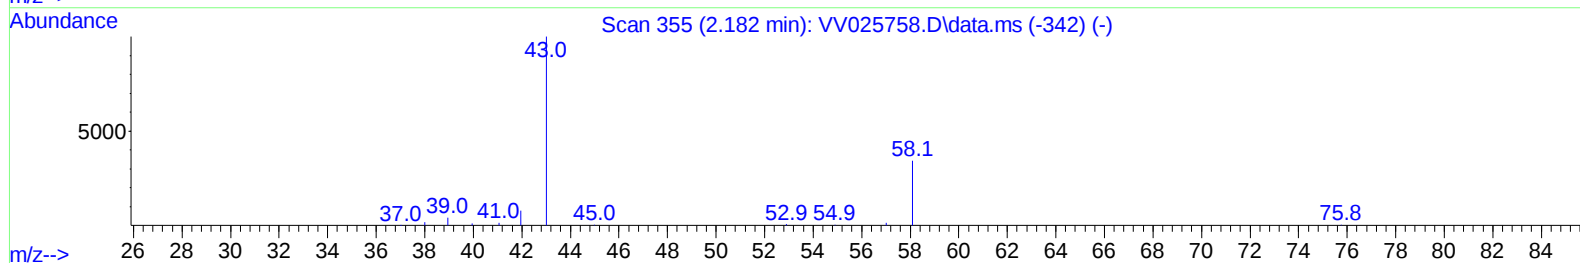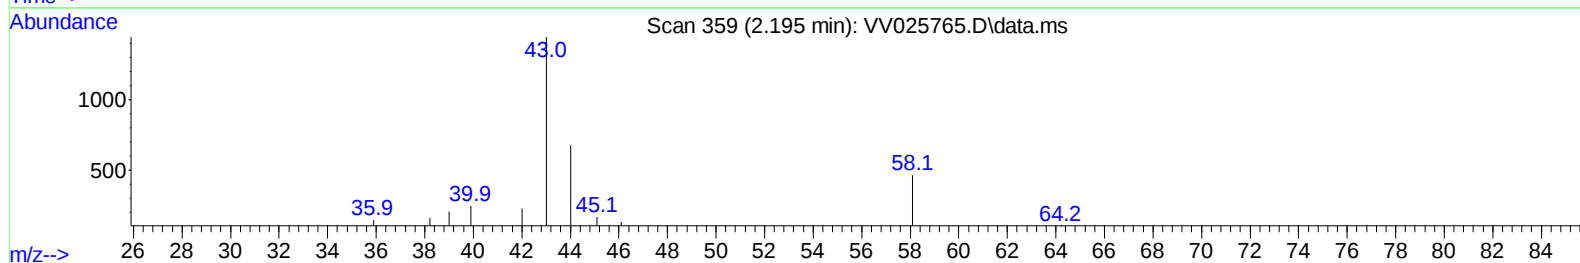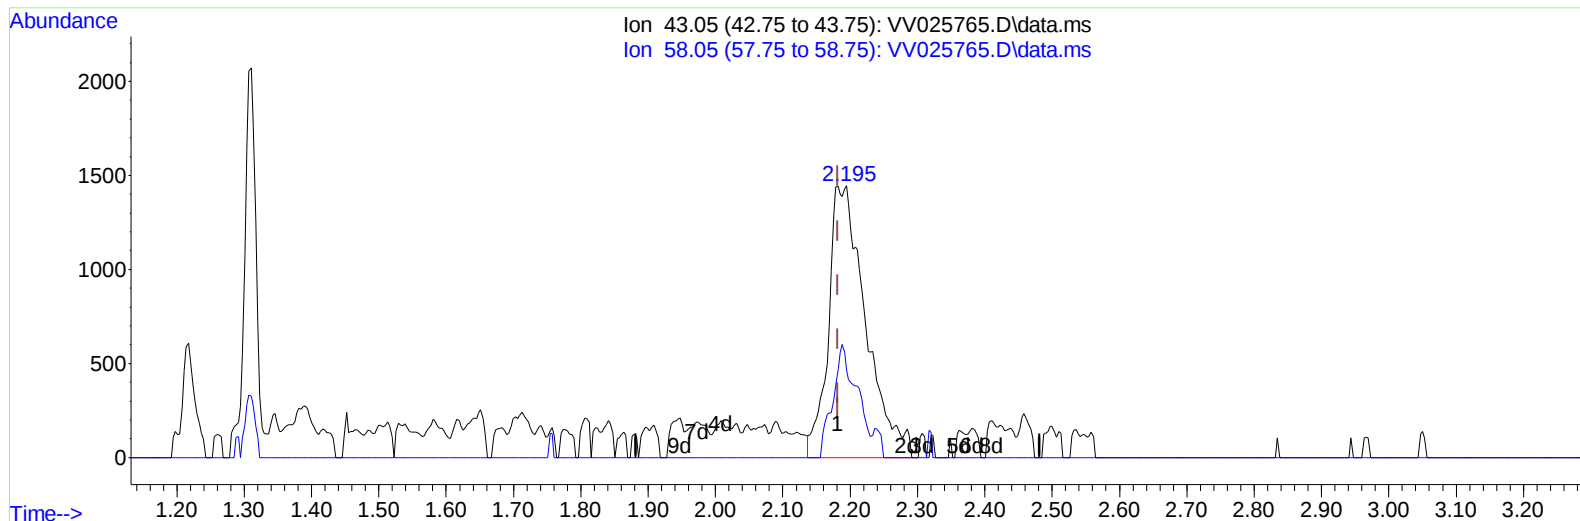

TIC: VV025765.D\data.ms

(13) Acetone (T)

2.195min (+ 0.013) 4.50 ug/L m

response 5531

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	36.10	26.72
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025765.D
 Acq On : 02 May 2022 14:57
 Operator : SY/MD
 Sample : N2621-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFJ8

Manual IntegrationsAPPROVED

Quant Time: May 03 05:24:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 03 05:22:31 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/09/2022
 Supervised By :Mahesh Dadoda 05/09/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	160269	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	160721	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	72667	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	45788	3.073	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	61.400%	
7) Chloroethane-d5	1.571	69	51670	3.260	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	65.200%	
11) 1,1-Dichloroethene-d2	2.111	63	76208	2.553	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	51.000%#	
20) 2-Butanone-d5	3.899	46	103781	57.259	ug/L	0.01
Spiked Amount 50.000	Range 40	- 130	Recovery	=	114.520%	
24) Chloroform-d	4.352	84	105029	4.665	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	93.200%	
26) 1,2-Dichloroethane-d4	5.037	65	49172	5.068	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	101.400%	
32) Benzene-d6	5.053	84	190740	4.102	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	82.000%	
36) 1,2-Dichloropropane-d6	6.069	67	61914	4.774	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	95.400%	
41) Toluene-d8	7.317	98	153078	3.547	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	71.000%	
43) trans-1,3-Dichloroprop...	7.629	79	13267	3.044	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	60.800%	
46) 2-Hexanone-d5	8.088	63	68951	45.069	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	90.140%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	41017	5.006	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	100.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	56819	4.664	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	93.200%	
Target Compounds						
					Qvalue	
13) Acetone	2.195	43	5531m	4.496	ug/L	
25) Chloroform	4.378	83	6282	0.302	ug/L	93
47) Tetrachloroethene	7.979	164	1304	0.132	ug/L	88
53) m,p-Xylene	9.149	106	1171	0.056	ug/L	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025765.D
Acq On : 02 May 2022 14:57
Operator : SY/MD
Sample : N2621-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFJ8

Manual IntegrationsAPPROVED

Quant Time: May 03 05:24:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 03 05:22:31 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/09/2022
Supervised By :Mahesh Dadoda 05/09/2022

