

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025759.D
 Acq On : 02 May 2022 12:31
 Operator : SY/MD
 Sample : VV0502WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK354

Quant Time: May 03 05:23:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 03 05:22:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	222640	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	224281	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	102409	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	112453	5.433	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	108.600%	
7) Chloroethane-d5	1.568	69	102917	4.674	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.400%	
11) 1,1-Dichloroethene-d2	2.108	63	162270	3.913	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	78.200%	
20) 2-Butanone-d5	3.886	46	131283	52.141	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	104.280%	
24) Chloroform-d	4.342	84	152677	4.881	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.600%	
26) 1,2-Dichloroethane-d4	5.027	65	68553	5.087	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.800%	
32) Benzene-d6	5.043	84	315370	4.860	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.200%	
36) 1,2-Dichloropropane-d6	6.063	67	91649	5.064	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	101.200%	
41) Toluene-d8	7.310	98	268781	4.463	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.200%	
43) trans-1,3-Dichloroprop...	7.619	79	25741	4.232	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	84.600%	
46) 2-Hexanone-d5	8.085	63	103651	48.550	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	97.100%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	52549	4.596	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	82931	4.830	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.600%	
Target Compounds						Qvalue
16) Methylene chloride	2.510	84	3832	0.205	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025759.D
Acq On : 02 May 2022 12:31
Operator : SY/MD
Sample : VV0502WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK354


Quant Time: May 03 05:23:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 03 05:22:31 2022
Response via : Initial Calibration

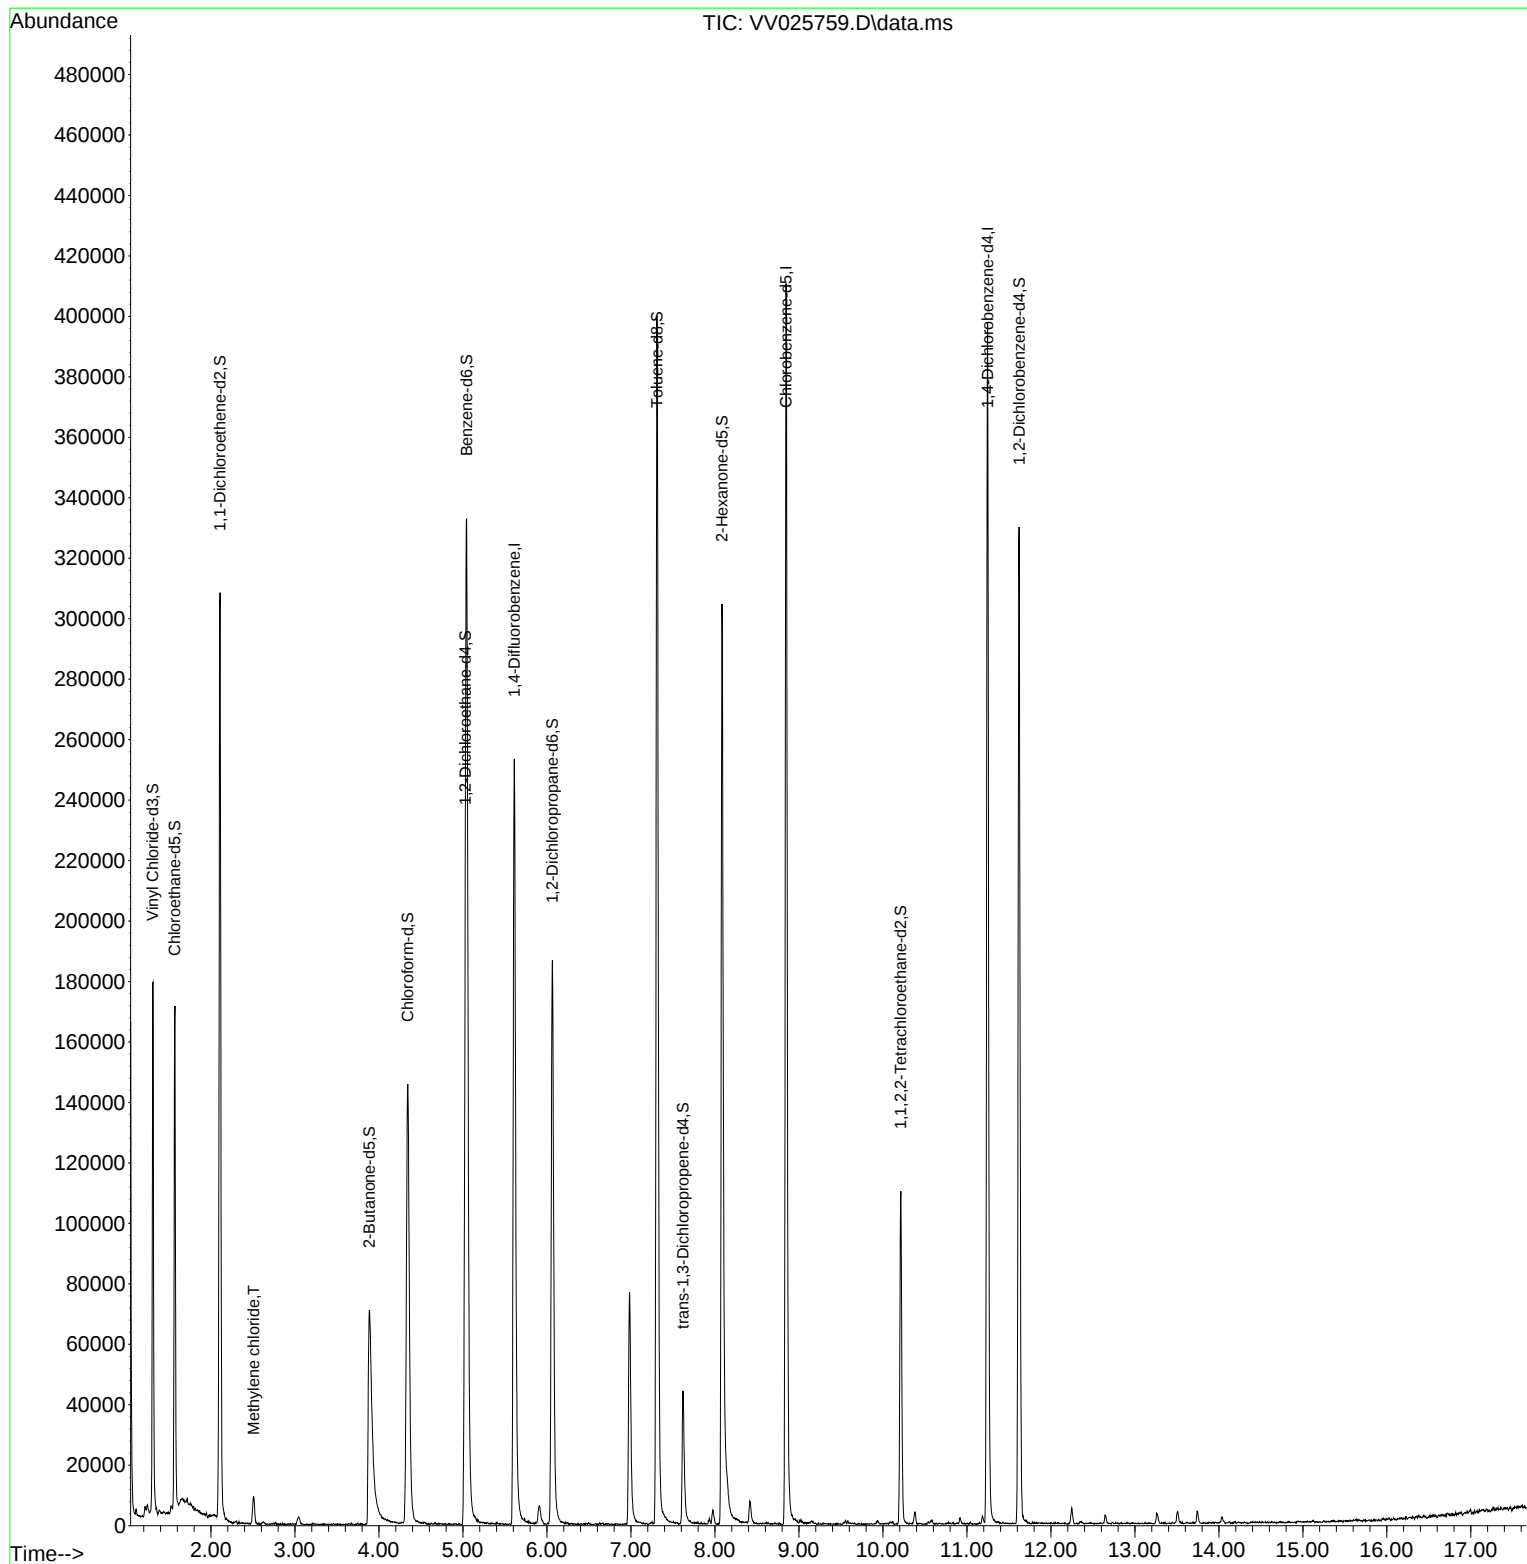

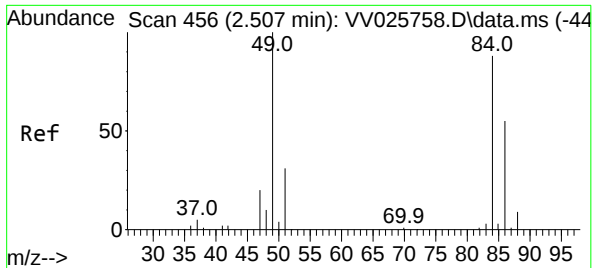

#16
Methylene chloride
Concen: 0.205 ug/L
RT: 2.510 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV025759.D
Acq: 02 May 2022 12:31

Instrument :
MSVOA_V
ClientSampleId :
VBLK354

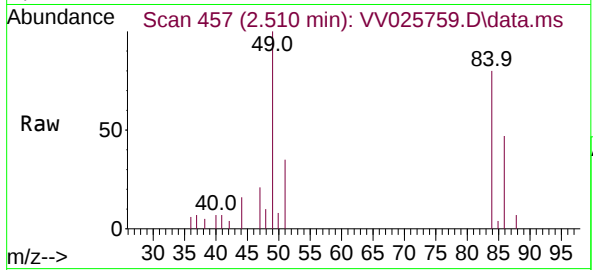

Tgt Ion:	84	Resp:	3832
Ion	Ratio	Lower	Upper
84	100		
86	59.2	45.9	85.3
49	125.0	76.6	142.3

