

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW050222\
 Data File : VW025760.D
 Acq On : 02 May 2022 13:00
 Operator : SY/MD
 Sample : N2612-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0C5

Quant Time: May 03 05:23:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 03 05:22:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	156361	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	160099	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	72738	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	46237	3.181	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	63.600%	
7) Chloroethane-d5	1.571	69	52031	3.364	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	67.200%	
11) 1,1-Dichloroethene-d2	2.111	63	76264	2.619	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	52.400%#	
20) 2-Butanone-d5	3.886	46	103771	58.685	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	117.360%	
24) Chloroform-d	4.346	84	103248	4.700	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.000%	
26) 1,2-Dichloroethane-d4	5.031	65	48061	5.078	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.600%	
32) Benzene-d6	5.047	84	194093	4.190	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	83.800%	
36) 1,2-Dichloropropane-d6	6.069	67	61374	4.751	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.000%	
41) Toluene-d8	7.313	98	154421	3.592	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	71.800%	
43) trans-1,3-Dichloroprop...	7.625	79	13540	3.118	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	62.400%	
46) 2-Hexanone-d5	8.085	63	74404	48.822	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	97.640%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	41009	5.025	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	100.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	57560	4.720	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	94.400%	
Target Compounds						Qvalue
47) Tetrachloroethene	7.979	164	6824	0.694	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025760.D
Acq On : 02 May 2022 13:00
Operator : SY/MD
Sample : N2612-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C5

Quant Time: May 03 05:23:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 03 05:22:31 2022
Response via : Initial Calibration

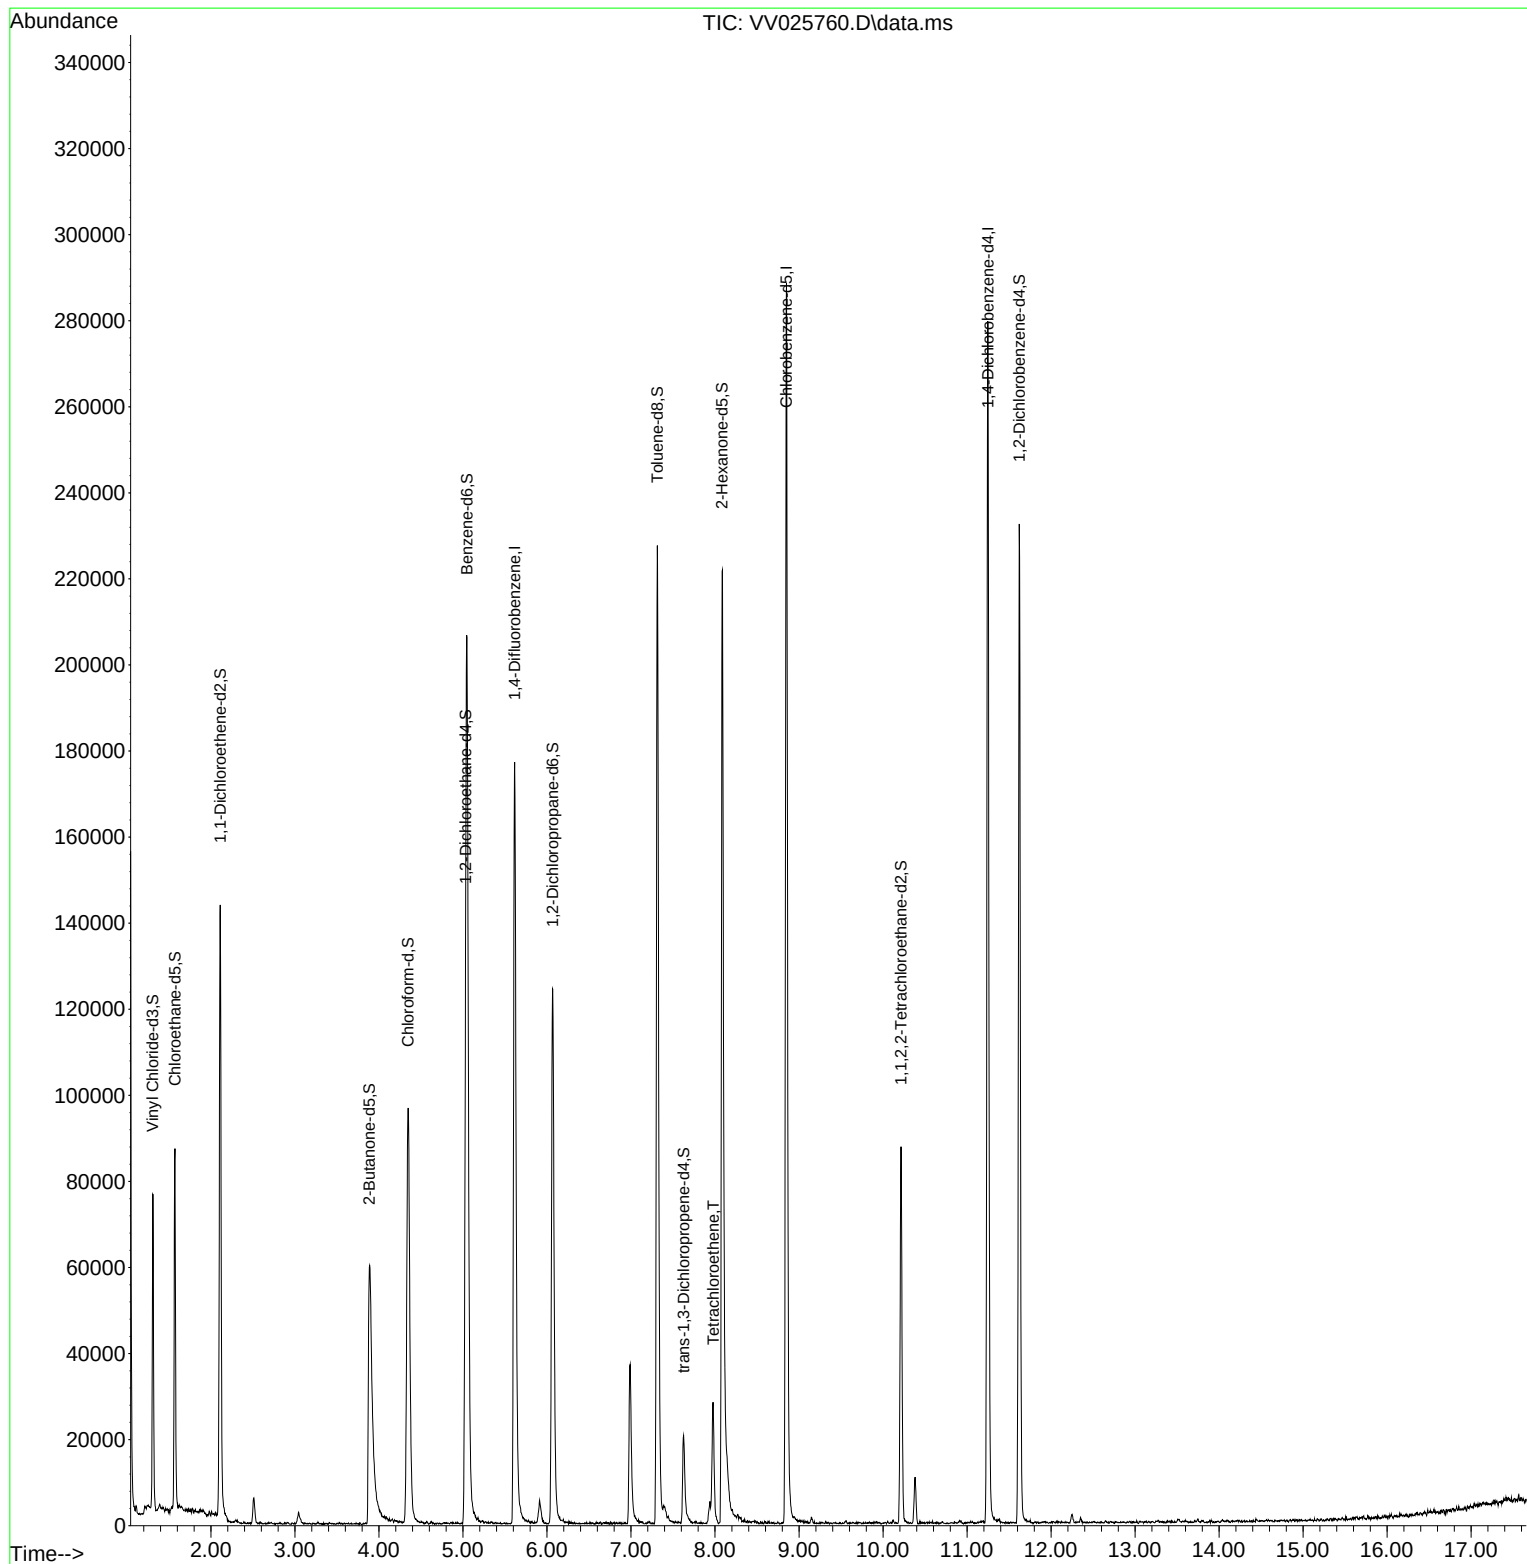

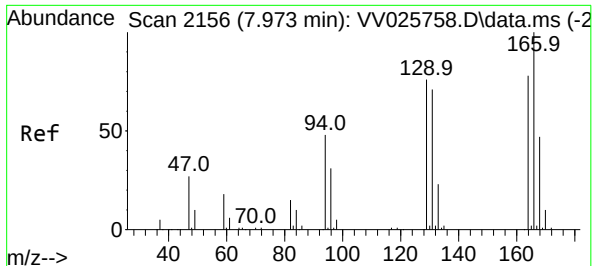

#47

Tetrachloroethene

Concen: 0.694 ug/L

RT: 7.979 min Scan# 21

Delta R.T. 0.006 min

Lab File: VV025760.D


Acq: 02 May 2022 13:00

Instrument :

MSVOA_V

ClientSampleId :

BH0C5

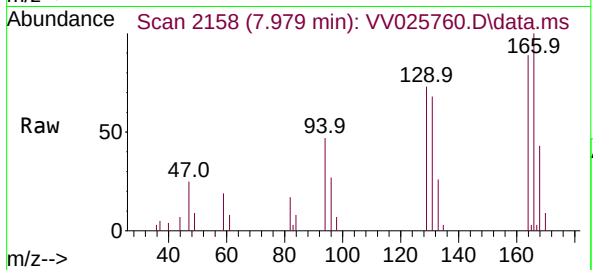

Tgt Ion:164 Resp: 6824

Ion Ratio Lower Upper

164 100

129 82.2 66.8 124.2

131 76.0 66.4 123.4

166 112.4 91.7 170.3

