

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW050222\
 Data File : VW025775.D
 Acq On : 02 May 2022 18:52
 Operator : SY/MD
 Sample : N2625-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW6Y0

Quant Time: May 03 05:26:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue May 03 05:22:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	144282	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	150387	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	61570	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	42712	3.184	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.600%
7) Chloroethane-d5	1.571	69	50291	3.524	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	70.400%
11) 1,1-Dichloroethene-d2	2.111	63	69545	2.588	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	51.800%#
20) 2-Butanone-d5	3.895	46	103015	63.134	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	126.260%
24) Chloroform-d	4.352	84	101402	5.003	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.000%
26) 1,2-Dichloroethane-d4	5.037	65	47519	5.441	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	108.800%
32) Benzene-d6	5.053	84	183700	4.222	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.400%
36) 1,2-Dichloropropane-d6	6.072	67	61258	5.048	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.000%
41) Toluene-d8	7.317	98	145713	3.609	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.200%
43) trans-1,3-Dichloroprop...	7.628	79	12822	3.144	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	62.800%
46) 2-Hexanone-d5	8.088	63	70588	49.310	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.620%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40776	5.319	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.400%
66) 1,2-Dichlorobenzene-d4	11.625	152	51829	5.021	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.400%
Target Compounds						Qvalue
14) Carbon disulfide	2.297	76	2452	0.082	ug/L	# 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025775.D
Acq On : 02 May 2022 18:52
Operator : SY/MD
Sample : N2625-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW6Y0


Quant Time: May 03 05:26:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue May 03 05:22:31 2022
Response via : Initial Calibration

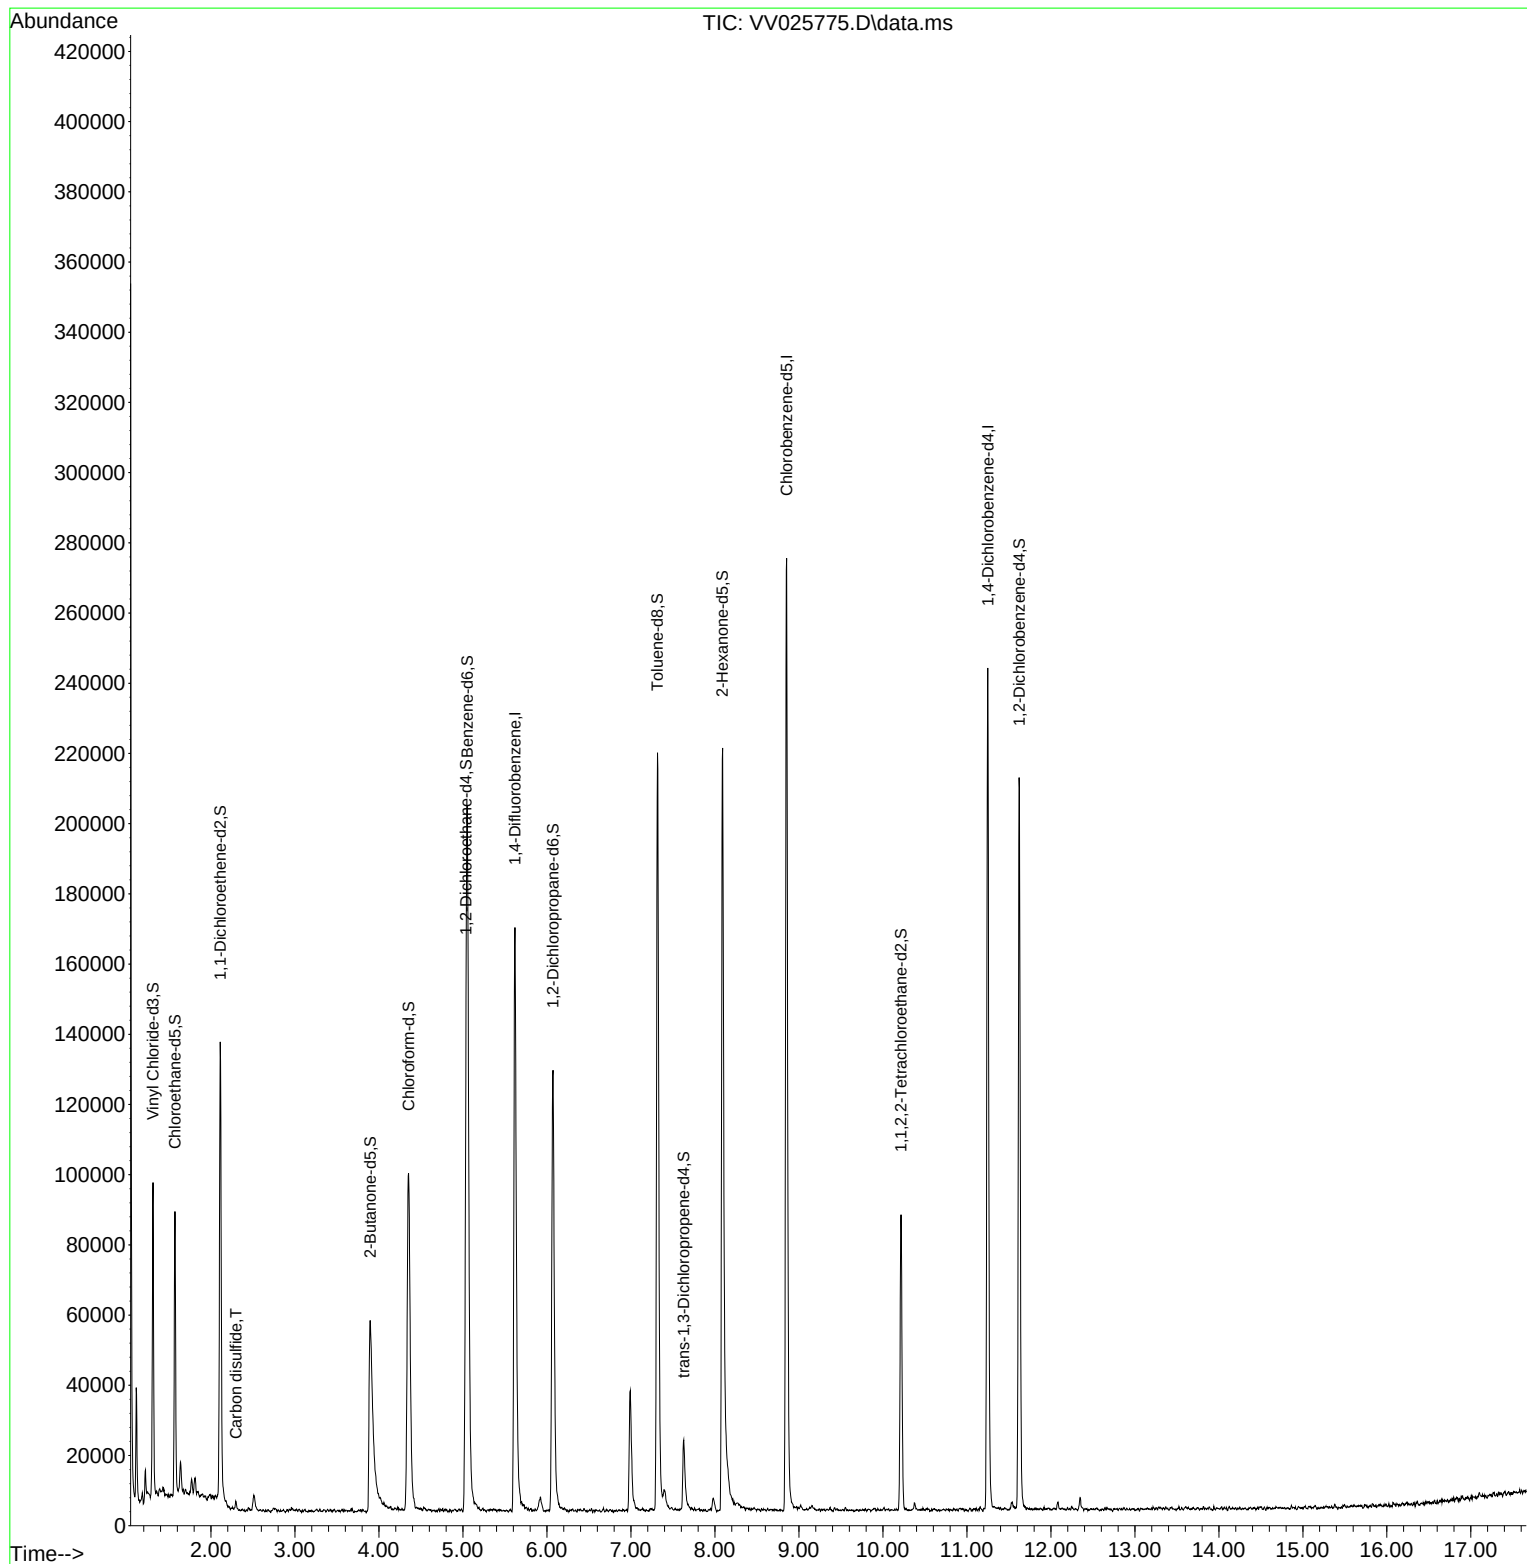

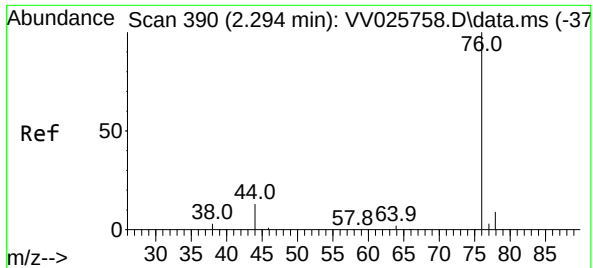

#14
Carbon disulfide
Concen: 0.082 ug/L
RT: 2.297 min Scan# 391
Delta R.T. 0.003 min
Lab File: VV025775.D
Acq: 02 May 2022 18:52

Instrument :
MSVOA_V
ClientSampleId :
EW6Y0

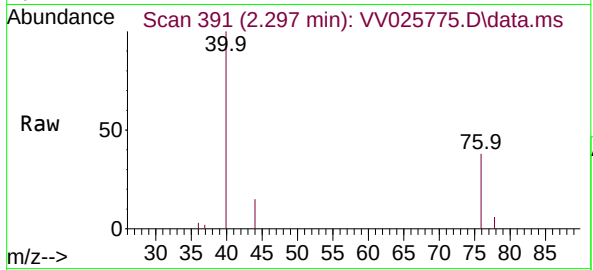

Tgt Ion: 76 Resp: 2452
Ion Ratio Lower Upper
76 100
78 15.6 7.3 10.9#

