

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025759.D
 Acq On : 02 May 2022 12:31
 Operator : SY/MD
 Sample : VV0502WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK354

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	75	84	95	rBV	174737	183399	22.12%	2.737%
2	1.571	156	165	178	rBV	166306	187245	22.58%	2.795%
3	2.108	320	332	352	rVB	306619	445055	53.67%	6.642%
4	2.506	445	456	465	rBV	9125	15938	1.92%	0.238%
5	3.886	875	885	926	rBV	70791	240923	29.05%	3.596%
6	4.342	1011	1027	1058	rBV2	145234	364813	44.00%	5.445%
7	5.043	1229	1245	1272	rBV2	332670	829197	100.00%	12.375%
8	5.612	1409	1422	1445	rBV	253197	520859	62.81%	7.774%
9	5.911	1504	1515	1532	rVB5	6147	14703	1.77%	0.219%
10	6.066	1548	1563	1594	rBV	186473	387522	46.73%	5.784%
11	6.982	1838	1848	1872	rBV2	76821	147368	17.77%	2.199%
12	7.310	1938	1950	1975	rBV	399397	703484	84.84%	10.499%
13	7.619	2036	2046	2068	rBV	43928	80378	9.69%	1.200%
14	8.085	2178	2191	2227	rBV	304449	582820	70.29%	8.698%
15	8.416	2285	2294	2305	rBV3	7138	11853	1.43%	0.177%
16	8.847	2416	2428	2449	rBV	410506	669137	80.70%	9.987%
17	10.214	2841	2853	2869	rBV	110134	175040	21.11%	2.612%
18	11.246	3163	3174	3197	rBV	396913	618440	74.58%	9.230%
19	11.622	3276	3291	3305	rBV	329665	522160	62.97%	7.793%




Sum of corrected areas: 6700334

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025759.D
Acq On : 02 May 2022 12:31
Operator : SY/MD
Sample : VV0502WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK354

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

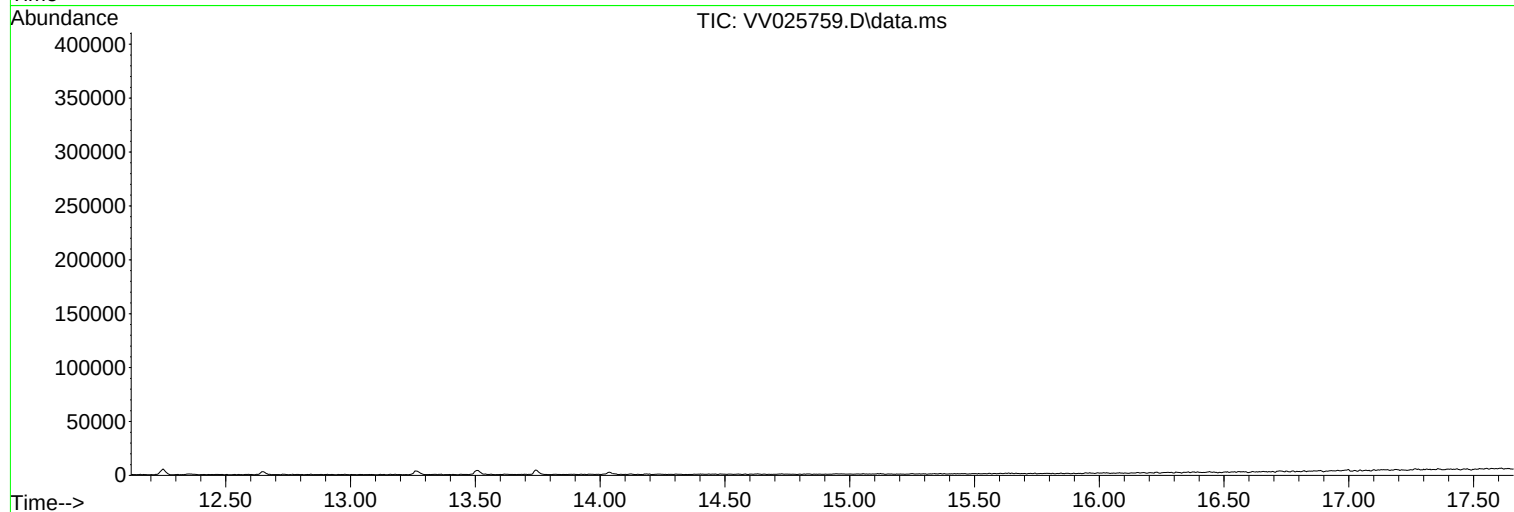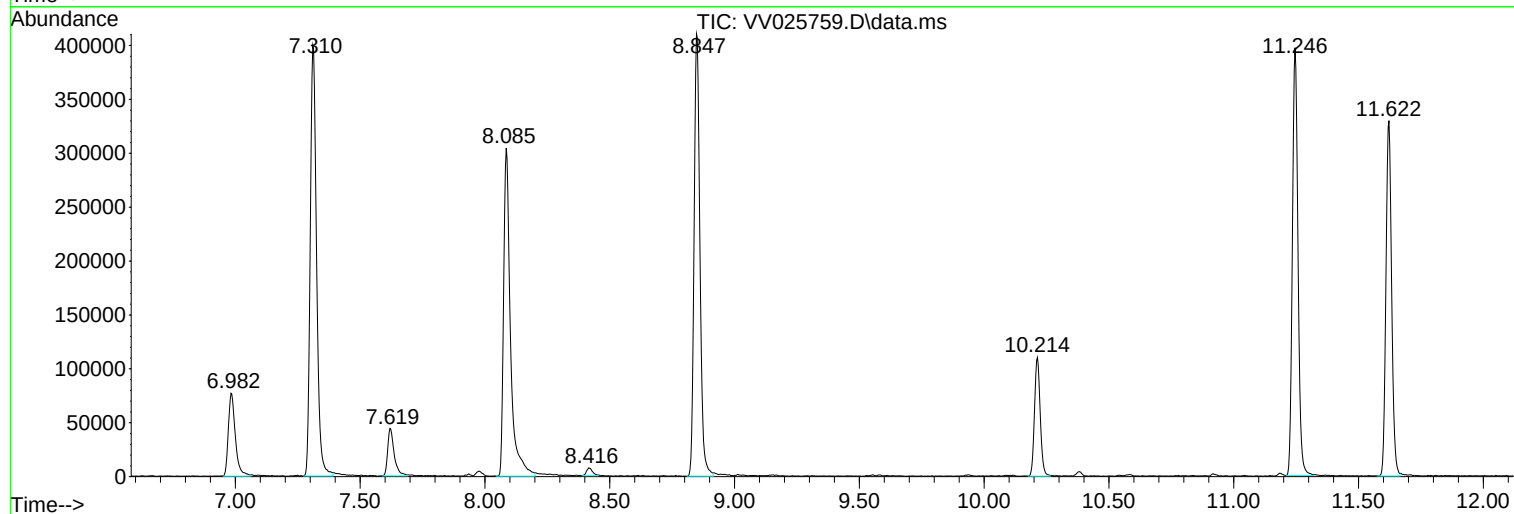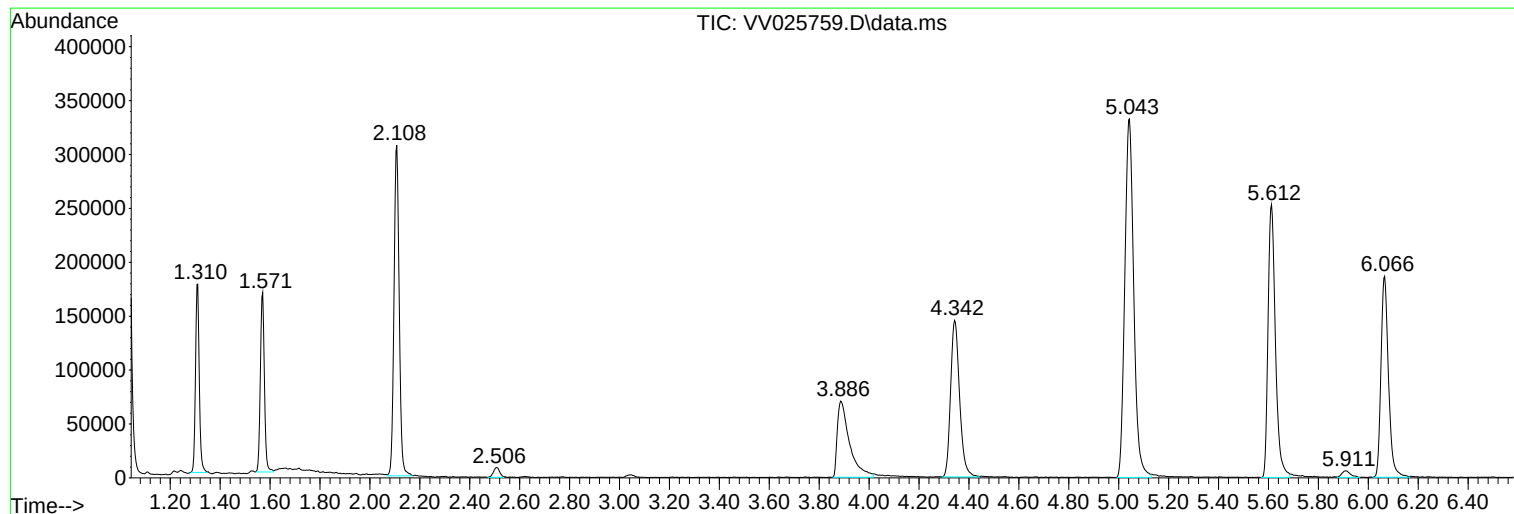

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025759.D
Acq On : 02 May 2022 12:31
Operator : SY/MD
Sample : VV0502WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK354

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025759.D
Acq On : 02 May 2022 12:31
Operator : SY/MD
Sample : VV0502WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK354

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc