

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025760.D
 Acq On : 02 May 2022 13:00
 Operator : SY/MD
 Sample : N2612-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0C5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025760.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rVB	73597	79423	15.15%	1.780%
2	1.571	157	165	179	rVB	83407	94341	18.00%	2.115%
3	2.111	319	333	346	rBV	141968	209316	39.93%	4.692%
4	2.510	446	457	466	rBV2	6121	10411	1.99%	0.233%
5	3.889	874	886	922	rBV2	60034	201234	38.39%	4.511%
6	4.349	1011	1029	1062	rBV2	96299	246805	47.08%	5.532%
7	5.043	1230	1245	1272	rBV2	206522	524250	100.00%	11.751%
8	5.616	1411	1423	1453	rBV	176815	366655	69.94%	8.219%
9	5.912	1501	1515	1528	rBV	5276	10722	2.05%	0.240%
10	6.066	1548	1563	1588	rBV	124292	262348	50.04%	5.881%
11	6.989	1840	1850	1866	rBV2	36991	72461	13.82%	1.624%
12	7.313	1939	1951	1971	rBV	227385	407997	77.82%	9.145%
13	7.625	2038	2048	2070	rBV3	20408	41446	7.91%	0.929%
14	7.940	2133	2146	2148	rBV3	5095	7360	1.40%	0.165%
15	7.976	2148	2157	2177	rVB2	28274	51739	9.87%	1.160%
16	8.088	2182	2192	2226	rBV	221361	437559	83.46%	9.808%
17	8.850	2418	2429	2452	rBV	288038	479088	91.39%	10.739%
18	10.214	2841	2853	2865	rBV	87503	136159	25.97%	3.052%
19	10.381	2893	2905	2917	rVB2	10860	17401	3.32%	0.390%
20	11.246	3163	3174	3196	rBV	279257	440455	84.02%	9.873%
21	11.622	3279	3291	3313	rBV	232235	364064	69.44%	8.161%




Sum of corrected areas: 4461234

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025760.D
Acq On : 02 May 2022 13:00
Operator : SY/MD
Sample : N2612-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

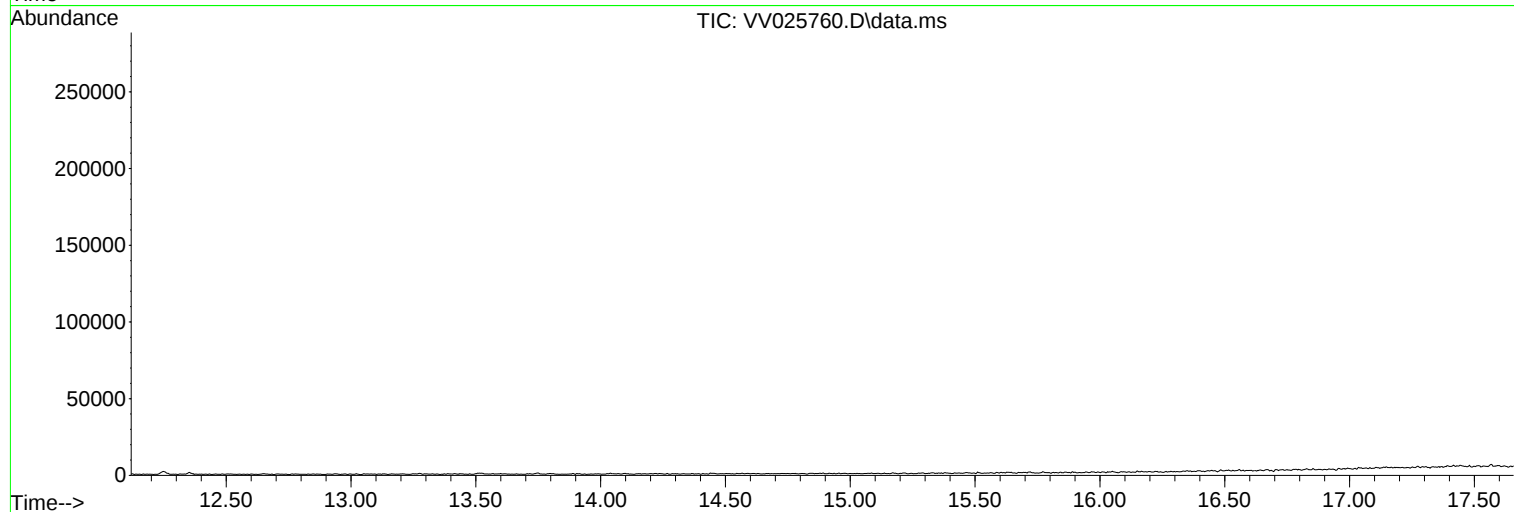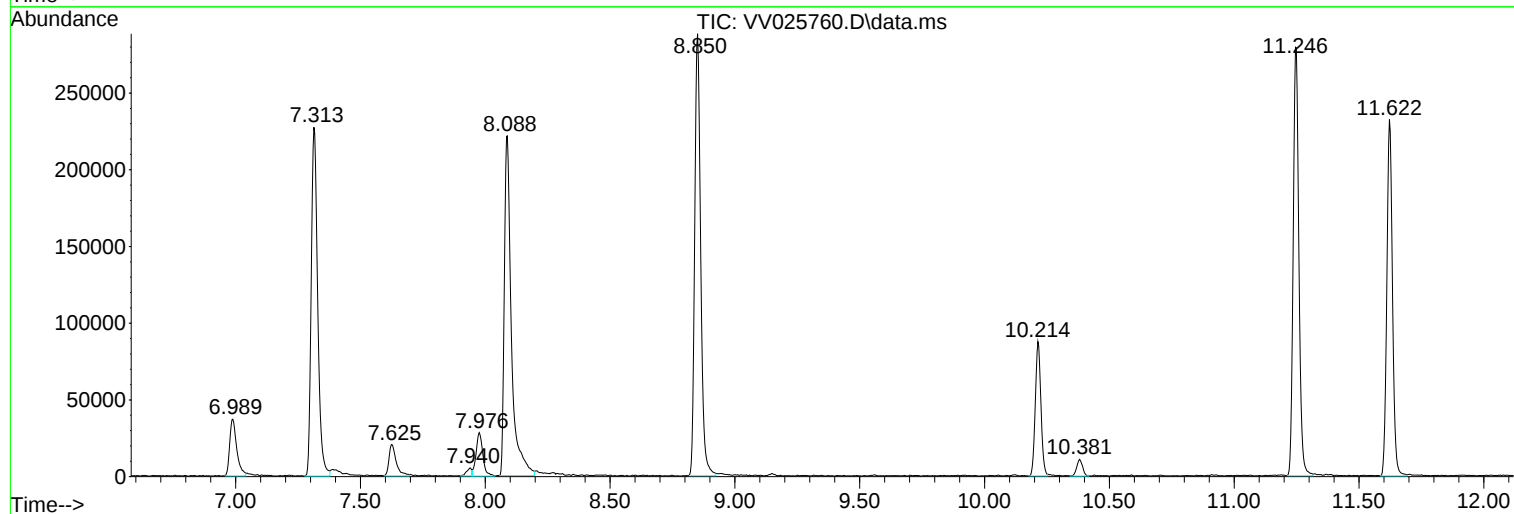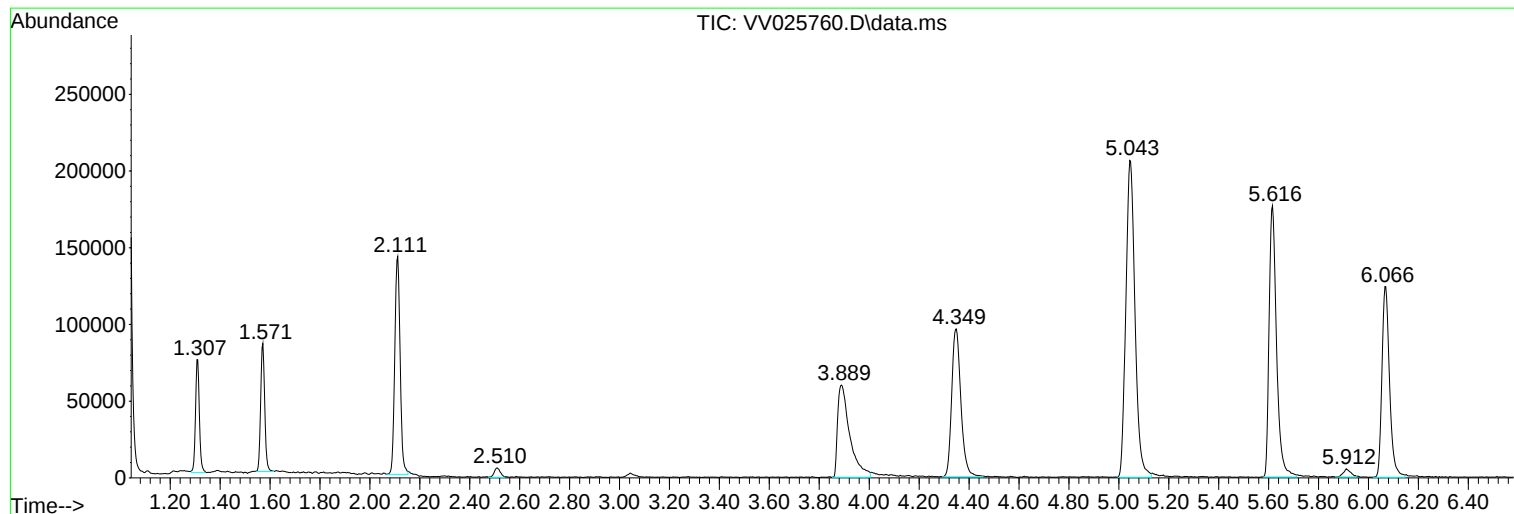

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025760.D
Acq On : 02 May 2022 13:00
Operator : SY/MD
Sample : N2612-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025760.D
Acq On : 02 May 2022 13:00
Operator : SY/MD
Sample : N2612-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc