

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025762.D
 Acq On : 02 May 2022 13:47
 Operator : SY/MD
 Sample : N2612-17
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH0C7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV025762.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	95	rVB	80436	83983	15.77%	1.863%
2	1.420	112	118	129	rVB	10664	12438	2.34%	0.276%
3	1.571	157	165	178	rBV	80768	92180	17.31%	2.045%
4	2.111	323	333	350	rVB	142383	210167	39.46%	4.662%
5	2.770	527	538	553	rBV4	6676	14648	2.75%	0.325%
6	3.902	875	890	925	rBV2	57980	218360	41.00%	4.843%
7	4.352	1012	1030	1056	rBV	99175	252818	47.46%	5.608%
8	5.050	1229	1247	1281	rBV2	208905	532649	100.00%	11.815%
9	5.619	1413	1424	1456	rBV2	176121	366825	68.87%	8.137%
10	6.072	1551	1565	1588	rBV	127693	267247	50.17%	5.928%
11	6.989	1839	1850	1873	rBV2	37007	72679	13.64%	1.612%
12	7.317	1941	1952	1972	rBV	236116	414249	77.77%	9.189%
13	7.628	2038	2049	2069	rBV	21194	41529	7.80%	0.921%
14	7.937	2136	2145	2151	rBV2	3478	5327	1.00%	0.118%
15	7.979	2151	2158	2168	rVB7	4575	7848	1.47%	0.174%
16	8.088	2182	2192	2227	rBV	230306	453264	85.10%	10.054%
17	8.850	2418	2429	2452	rBV	296269	486902	91.41%	10.800%
18	10.214	2842	2853	2871	rBV	90977	147038	27.61%	3.261%
19	10.381	2896	2905	2916	rBV3	6504	10614	1.99%	0.235%
20	11.246	3163	3174	3198	rBV	289510	450167	84.51%	9.985%
21	11.622	3280	3291	3308	rBV	233360	367389	68.97%	8.149%




Sum of corrected areas: 4508321

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025762.D
Acq On : 02 May 2022 13:47
Operator : SY/MD
Sample : N2612-17
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

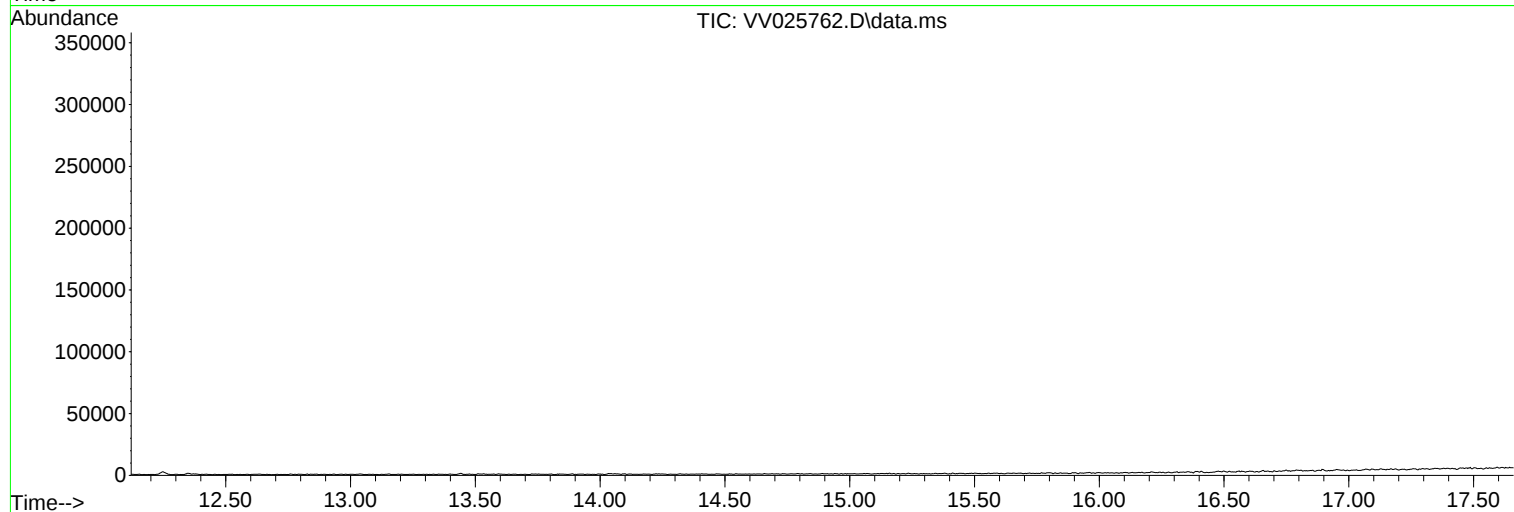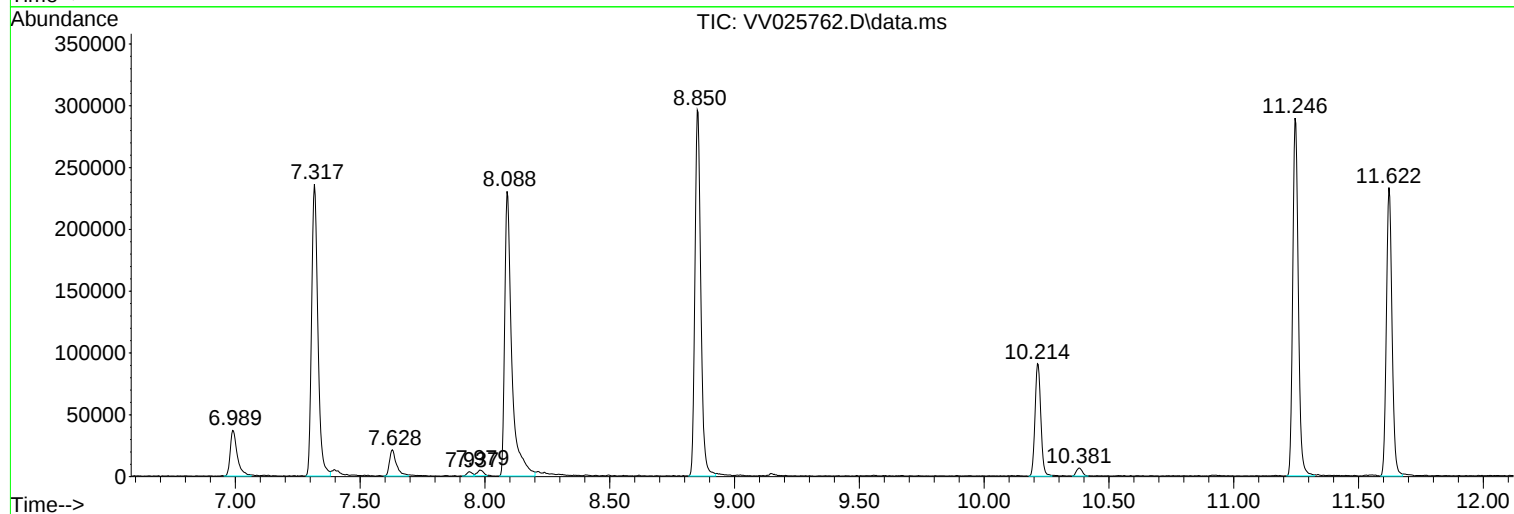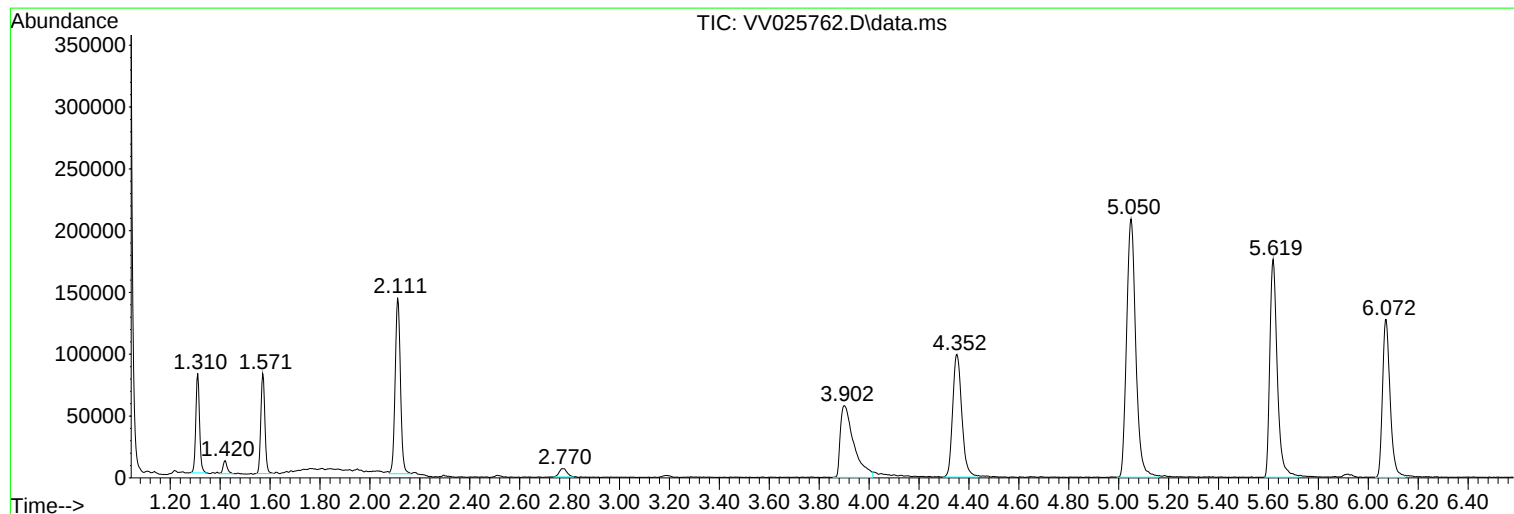

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025762.D
Acq On : 02 May 2022 13:47
Operator : SY/MD
Sample : N2612-17
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025762.D
Acq On : 02 May 2022 13:47
Operator : SY/MD
Sample : N2612-17
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH0C7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc