

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025763.D
 Acq On : 02 May 2022 14:10
 Operator : SY/MD
 Sample : N2621-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFJ6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025763.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	76	84	94	rBV	80571	81793	15.27%	1.823%
2	1.571	157	165	175	rBV	83874	95381	17.80%	2.126%
3	2.111	323	333	344	rBV	144518	207320	38.70%	4.620%
4	3.902	879	890	917	rBV2	50887	174660	32.60%	3.893%
5	4.352	1014	1030	1058	rBV2	101196	263802	49.24%	5.879%
6	5.050	1230	1247	1274	rBV2	211863	535770	100.00%	11.940%
7	5.619	1412	1424	1452	rBV	174730	359127	67.03%	8.004%
8	6.069	1552	1564	1591	rBV2	128526	267613	49.95%	5.964%
9	6.989	1840	1850	1876	rBV2	37689	76147	14.21%	1.697%
10	7.317	1940	1952	1970	rBV	229716	411163	76.74%	9.163%
11	7.397	1970	1977	1989	rVB3	6779	13762	2.57%	0.307%
12	7.625	2039	2048	2068	rBV2	21379	42729	7.98%	0.952%
13	7.979	2151	2158	2170	rVB7	4471	7283	1.36%	0.162%
14	8.092	2183	2193	2235	rBV2	220962	455571	85.03%	10.153%
15	8.850	2418	2429	2454	rBV	287438	478030	89.22%	10.654%
16	9.146	2511	2521	2534	rBV3	3406	6547	1.22%	0.146%
17	10.214	2841	2853	2870	rBV	87538	140430	26.21%	3.130%
18	10.381	2894	2905	2914	rBV3	7172	10722	2.00%	0.239%
19	11.246	3161	3174	3194	rBV	274338	432626	80.75%	9.642%
20	11.532	3256	3263	3275	rBV6	6214	10643	1.99%	0.237%
21	11.622	3280	3291	3307	rBV	231258	361889	67.55%	8.065%
22	12.249	3476	3486	3498	rVB3	3874	6183	1.15%	0.138%
23	12.342	3505	3515	3529	rBV2	30484	47864	8.93%	1.067%




Sum of corrected areas: 4487055

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025763.D
Acq On : 02 May 2022 14:10
Operator : SY/MD
Sample : N2621-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

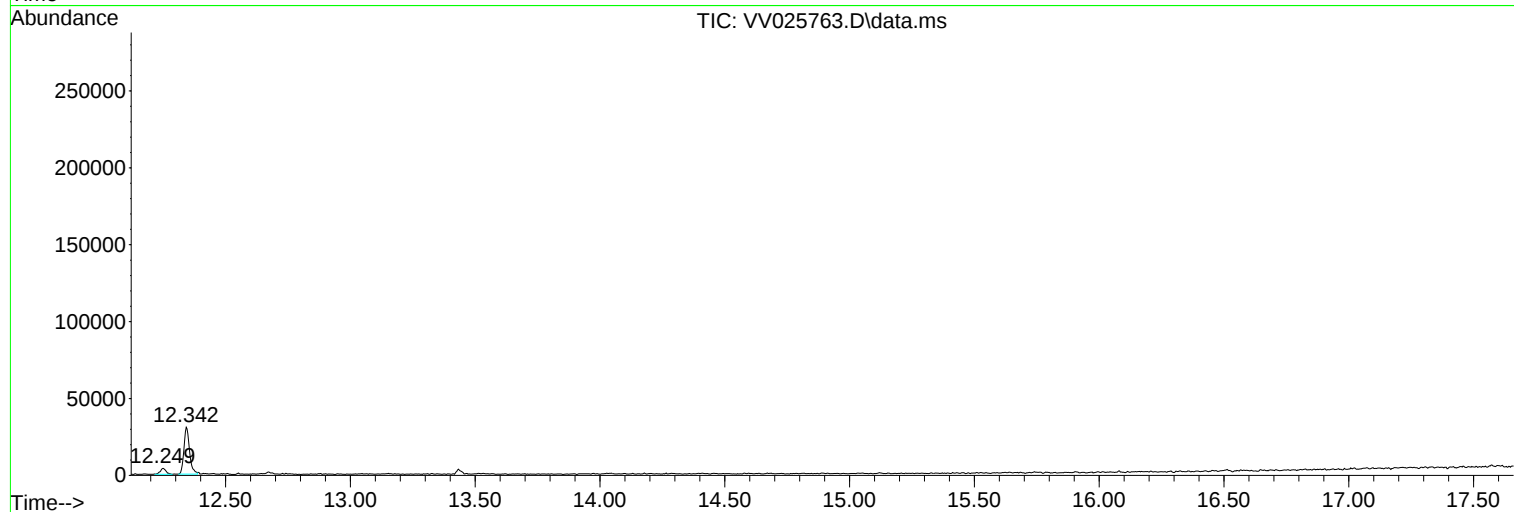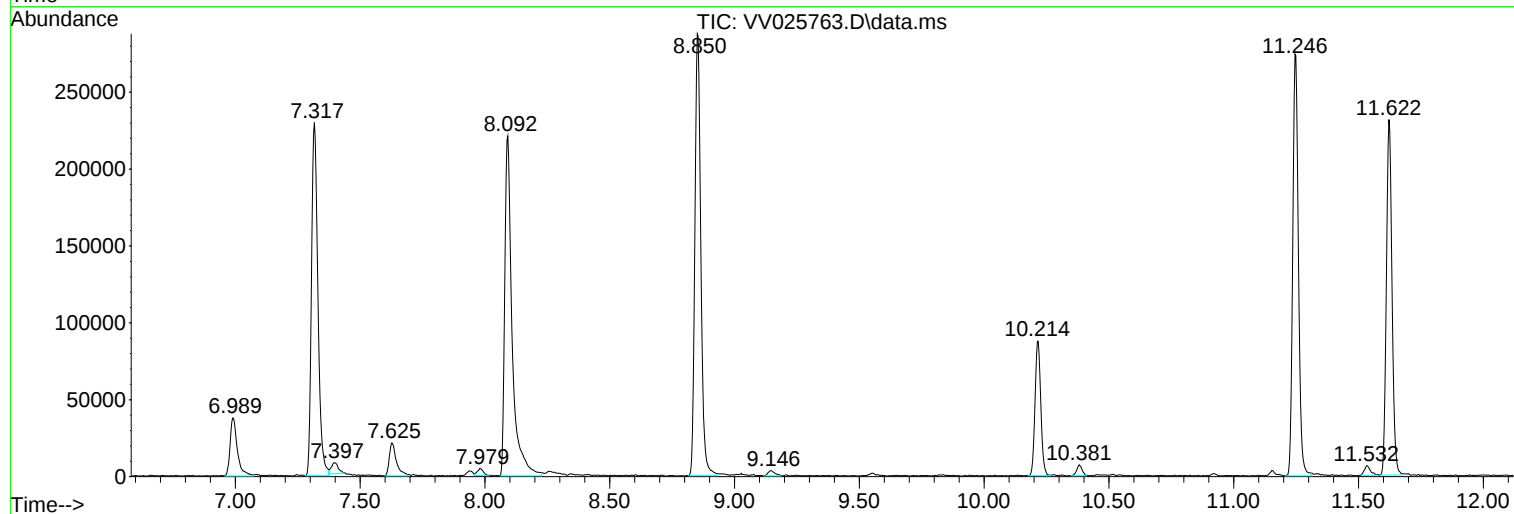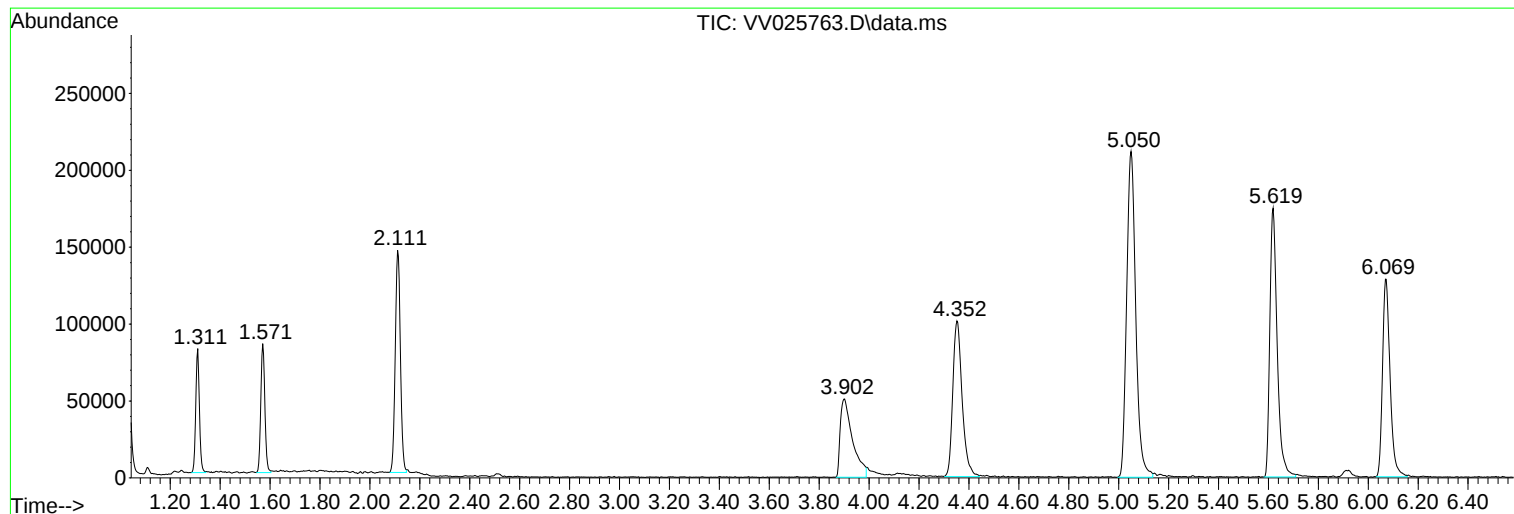

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025763.D
Acq On : 02 May 2022 14:10
Operator : SY/MD
Sample : N2621-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFJ6










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.342	0.55 ug/L	47864	1,4-Dichlorobenzene-d4	11.249

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclohexanol, 2-methyl-	114	C7H14O	000583-59-5	38
2			Cycloheptane	98	C7H14	000291-64-5	35
3			Cyclohexanol, 2-methyl-, trans-	114	C7H14O	007443-52-9	30
4			Cyclohexanol, 2-methyl-, cis-	114	C7H14O	007443-70-1	30
5			Cyclooctyl alcohol	128	C8H16O	000696-71-9	27

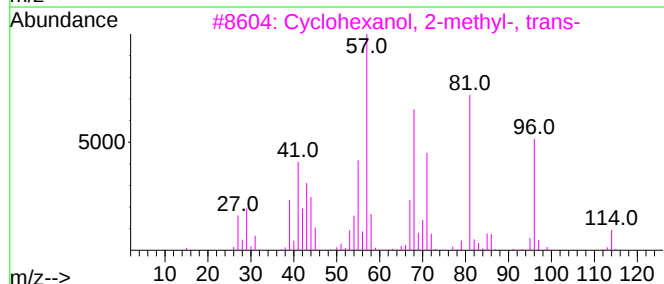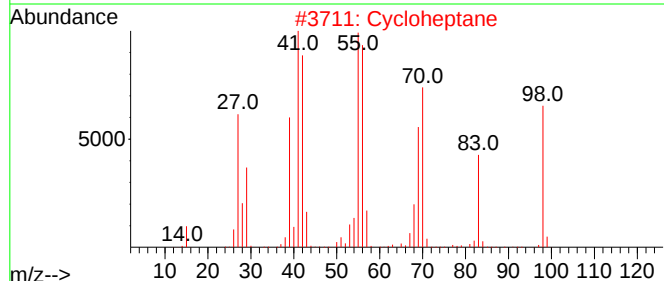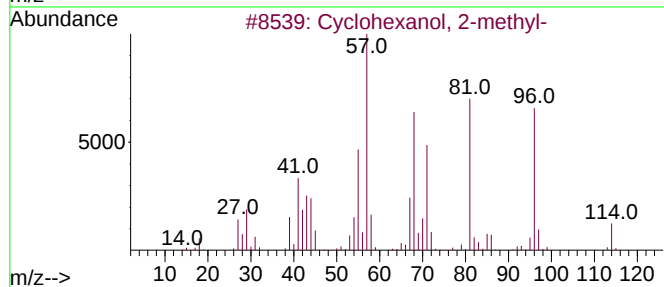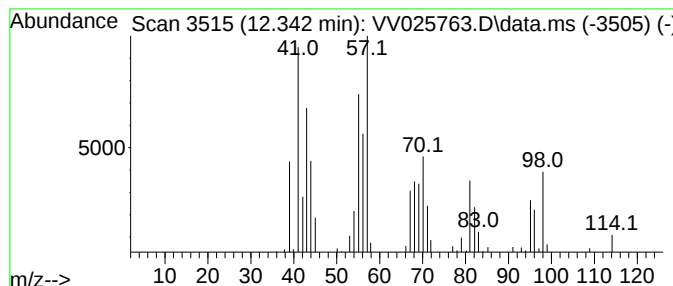

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025763.D
Acq On : 02 May 2022 14:10
Operator : SY/MD
Sample : N2621-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	12.342	0.6	ug/L	47864	3	11.249	432626	5.0