

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
 Data File : VV025766.D
 Acq On : 02 May 2022 15:21
 Operator : SY/MD
 Sample : N2621-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFFJ0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV025766.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	76	84	93	rVB	79204	78472	14.69%	1.773%
2	1.571	157	165	175	rBV	83364	93025	17.42%	2.101%
3	2.111	322	333	345	rBV	146459	208684	39.08%	4.714%
4	3.899	878	889	924	rBV	48826	178959	33.51%	4.043%
5	4.352	1012	1030	1061	rBV	101472	260140	48.71%	5.877%
6	5.050	1231	1247	1276	rBV2	207064	534022	100.00%	12.064%
7	5.619	1412	1424	1447	rBV	179661	368761	69.05%	8.331%
8	5.915	1503	1516	1521	rBV8	5359	9777	1.83%	0.221%
9	6.072	1552	1565	1592	rBV	127590	267997	50.18%	6.054%
10	6.992	1840	1851	1870	rBV2	38896	74940	14.03%	1.693%
11	7.317	1940	1952	1971	rBV	234065	412414	77.23%	9.317%
12	7.625	2039	2048	2068	rBV2	22356	41758	7.82%	0.943%
13	7.979	2151	2158	2171	rVB4	6266	10450	1.96%	0.236%
14	8.092	2183	2193	2231	rBV	218849	450903	84.44%	10.186%
15	8.854	2417	2430	2453	rBV	293070	486883	91.17%	10.999%
16	10.214	2843	2853	2870	rBV	86669	137455	25.74%	3.105%
17	10.381	2897	2905	2917	rBV2	6783	11165	2.09%	0.252%
18	11.246	3163	3174	3196	rBV	277763	438262	82.07%	9.901%
19	11.622	3280	3291	3307	rBV	228328	362544	67.89%	8.190%




Sum of corrected areas: 4426611

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025766.D
Acq On : 02 May 2022 15:21
Operator : SY/MD
Sample : N2621-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

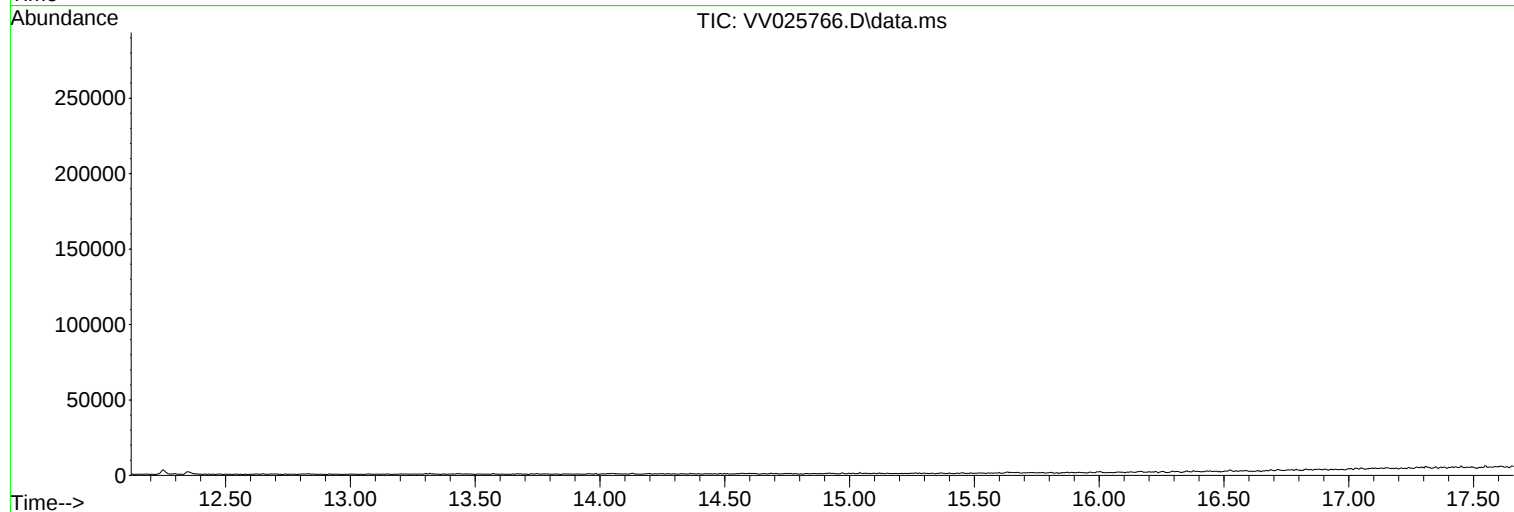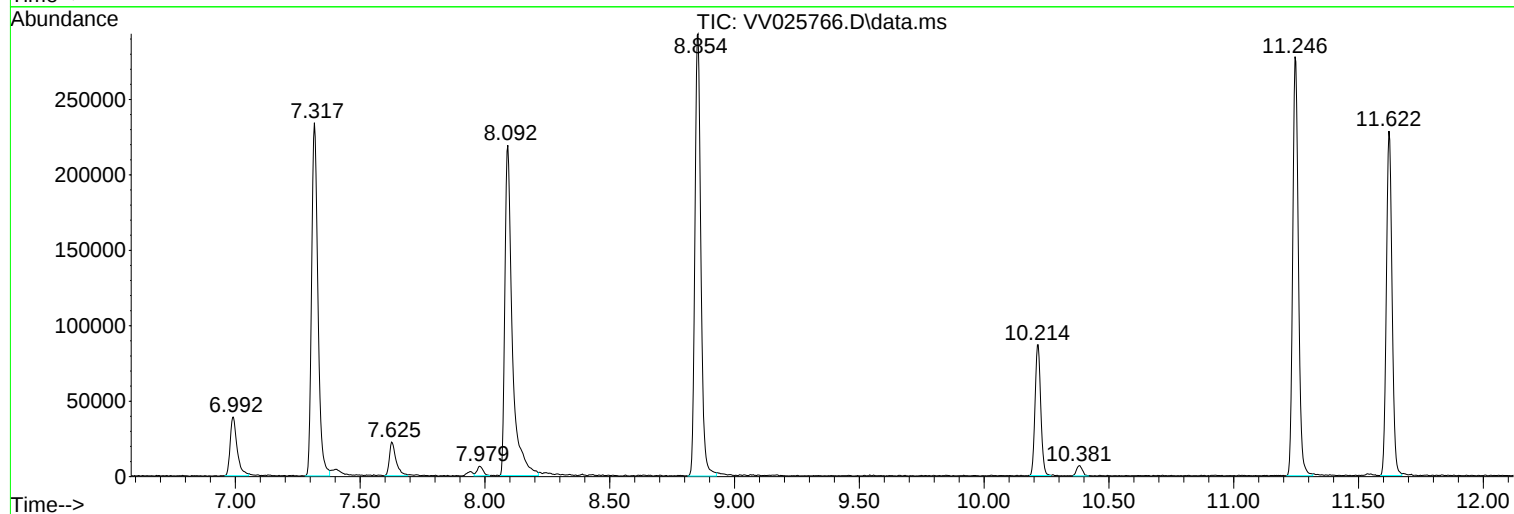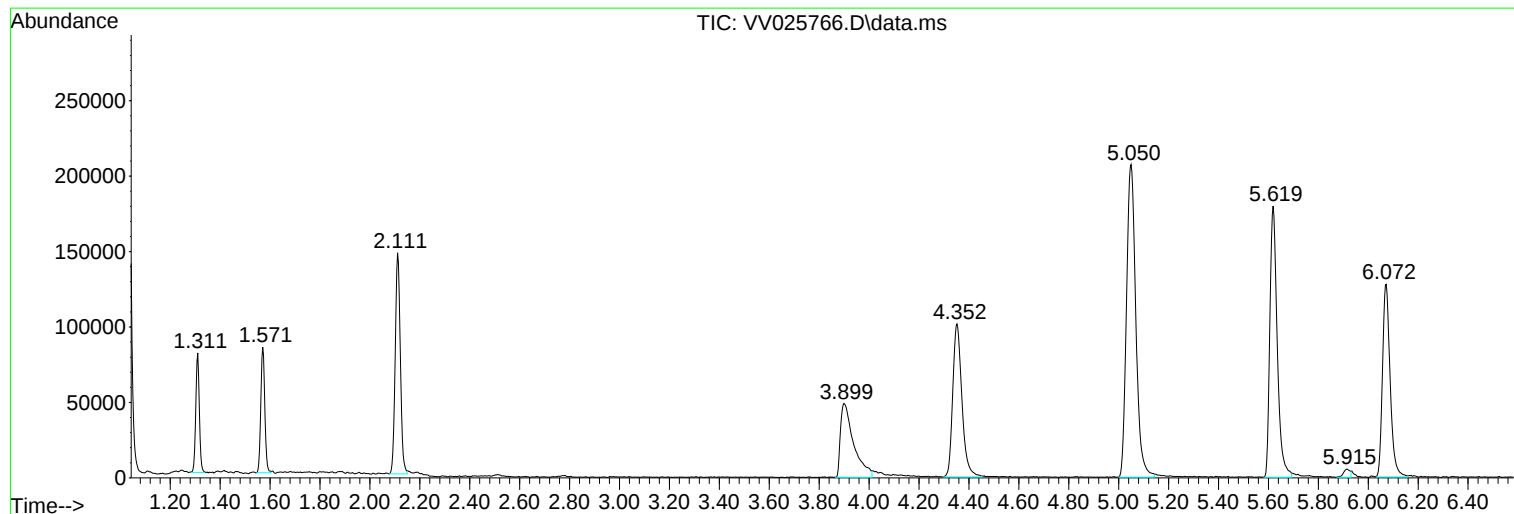

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025766.D
Acq On : 02 May 2022 15:21
Operator : SY/MD
Sample : N2621-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV050222\
Data File : VV025766.D
Acq On : 02 May 2022 15:21
Operator : SY/MD
Sample : N2621-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFFJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR040822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc